

An Open-Source Environmental Chamber for Materials-Stability Testing Using an Optical Proxy

Rodolfo Keesey^{*,§,1}, Armi Tiihonen^{**,§,2,3}, Alexander E. Siemenn³, Thomas W. Colburn⁴, Shijing Sun³, Noor Titan Putri Hartono³, James Serdy³, Margaret Zeile¹, Keqing He¹, Cole A. Gurtner⁴, Austin C. Flick⁴, Clio Batali³, Alex Encinas³, Richa R. Naik³, Zhe Liu³, Felipe Oviedo³, I. Marius Peters³, Janak Thapa³, Siyu Isaac Parker Tian⁵, Reinhold H. Dauskardt⁴, Alexander J. Norquist^{***,1}, Tonio Buonassisi^{****,3}

* rkeesey@fordham.edu
** armi.tiihonen@gmail.com
*** anorquis@haverford.edu
**** buonassi@mit.edu

§ Contributed equally

¹ Haverford College, 370 Lancaster Avenue, Haverford, 19041, Pennsylvania, USA

² Department of Applied Physics, Aalto University, P.O. Box 11100, Aalto, FI-00076, Finland

³ Massachusetts Institute of Technology, Cambridge, MA 02139, USA

⁴ Department of Materials Science and Engineering, Stanford University, Stanford, CA 94305, USA

⁵ Low Energy Electronic Systems (LEES), Singapore-MIT Alliance for Research and Technology (SMART), Singapore 138602, Singapore

Abstract

This study is motivated by the desire to disseminate a low-cost, high-precision, high-throughput environmental chamber to test materials and devices under elevated humidity, temperature, and light. This paper documents the creation of an open-source tool with a bill of materials as low as US\$2,000, and the subsequent evolution of three second-generation tools installed at three different universities spanning thin films, bulk crystals, and thin-film solar-cell devices. We introduce an optical proxy measurement to detect real-time phase changes in materials. We present correlations between this optical proxy and standard X-ray diffraction measurements, describe some edge cases where the proxy measurement fails, and report key learnings from the technology-translation process. By sharing lessons learned, we hope that future open-hardware development and translation efforts can proceed with reduced friction. Throughout the paper, we provide examples of scientific impact, wherein participating laboratories used their environmental chambers to study and improve the stabilities of halide-perovskite materials. All generations of hardware bills of materials, assembly instructions, and operating codes are available in open-source repositories.

1. Introduction

Quantifying and predicting long-term stability in realistic operating environments is of interest to a broad range of materials, from energy devices to marine and offshore environments [1]–[5]. However, accelerated environmental testing today is often time-intensive and expensive, limiting

the speed of materials innovation. Commercial stability chambers can cost tens of thousands of US dollars, and may require additional modification to generate consistent-quality degradation data for a specific application [6]. Given the rise of automated experimentation systems and artificial intelligence in materials discovery [7]–[9], developing stability testing equipment that can both mitigate the cost of longitudinal testing and provide high quality, machine-interpretable degradation data grows in importance, addressing a bottleneck in high-throughput materials discovery.

To meet this need, we introduce a low-cost, open-source environmental chamber. Commercial environmental chambers that control temperature and humidity can cost over US \$10,000, and fully integrated solar device stability testing systems can cost up to US \$60,000. Our chambers range from US \$2,000–\$7,500 depending on configuration, and offer environmental control as well as in-situ monitoring. Although the design principles of the chamber are broadly applicable, we designed the chamber specifically to test halide perovskites, a class of functional materials with nascent applications including photovoltaic absorbers, light-emitting devices, and X-ray detectors, among others [10], [11]. Commercialization of the aforementioned devices is often limited by poor environmental stability under operating conditions [12]–[16]. This has led to diverse efforts to modify perovskite alloy composition and device architecture [17], with the aim of improving environmental stability and widening accessibility by reducing price. The extent and mechanism by which newly synthesized alloys and devices degrade under environmental conditions is a subject for study [18]–[20].

We designed this open-source hardware platform to be easily reconfigurable to a range of materials and form factors. To test this flexibility of the principles of construction and operation of the environmental chamber, we report the original hardware design suitable for testing bare thin films, and also three subsequent equipment modifications, including adaptations to study either perovskite devices or bulk crystals. Two of these modifications occurred in different laboratories. We report key learnings from this technology translation process with the goal of defining a set of best practices for open hardware reporting. We observe that open hardware is common for foundational chemical tasks (*i.e.*, liquid handling [21]–[24]) but has been slower to realize for more specialized tasks like stability testing. Ideally, sharing these learnings may expedite the processes of creating and adapting future specialized open hardware.

Another key element to high-throughput testing is the development and validation of proxy measurement techniques. We posit that the many physically- and chemically-meaningful signals have optical signatures that are often overlooked. Here, we use a visible-light camera as a proxy for perovskite phase transitions, validate this proxy using X-ray diffraction (XRD), and describe the limits under which this proxy measurement is valid. Using an optical proxy for stability accelerates the rate of data acquisition by more than an order of magnitude and enables low-cost *in-situ* measurements during environmental degradation.

In summary, we report an open-source aging chamber design, designed for high-throughput, semi-automated stability measurements of perovskite samples. This article is structured as follows: First, we establish the design principles of the environmental chamber and present evidence for perovskite color change being a suitable proxy for perovskite degradation, and determine the limits of proxy validity. Second, we describe the chamber versions. Third, we discuss our process of

open-hardware dissemination between three different laboratories, and identify principles that may facilitate similar efforts in the future. By firstly sharing all the three designs and secondly discussing the development process itself, we hope to encourage wider adoption of specialized open-hardware efforts in materials research, and facilitate further evolution of this environmental chamber design in new applications and laboratories.

2. Conception

2a. Generating machine-compatible stability data

An open-hardware design for an environmental chamber was originally conceived at MIT to leverage community inputs and refinements in subsequent generations. The build guide was shared with collaborators, and the hardware design evolved into a second generation in parallel efforts at three different sites (Figure 1): Haverford (Norquist laboratory), Stanford (Dauskardt laboratory), and the original MIT group (Buonassisi laboratory).

Our hardware-design goal was to generate machine compatible degradation data to aid halide-perovskite stability research. We wanted the degradation chamber to fulfill four intertwined requirements to reach machine compatibility: The ideal device should be capable of producing degradation data with sufficiently high throughput for the machine learning algorithms. Linked to this requirement, the device should be low cost to enable expansion when necessary. Experimental variance can lead to erroneous conclusions, especially in high-throughput experimental workflows guided by machine learning, (garbage in, garbage out). Thus, the data should have low variations and preferably no physical contacts to the samples.

These criteria require judicious selection of the response variable for the in-situ degradation system. Direct observations of phase transformations via XRD normally require removing samples from the aging chamber, perturbing the aging process. In situ electrical measurements provide useful information, but require electric contacts that can be prone to (intermittent) faults. Thus, we opted for a non-invasive optical signature as a proxy for sample degradation.

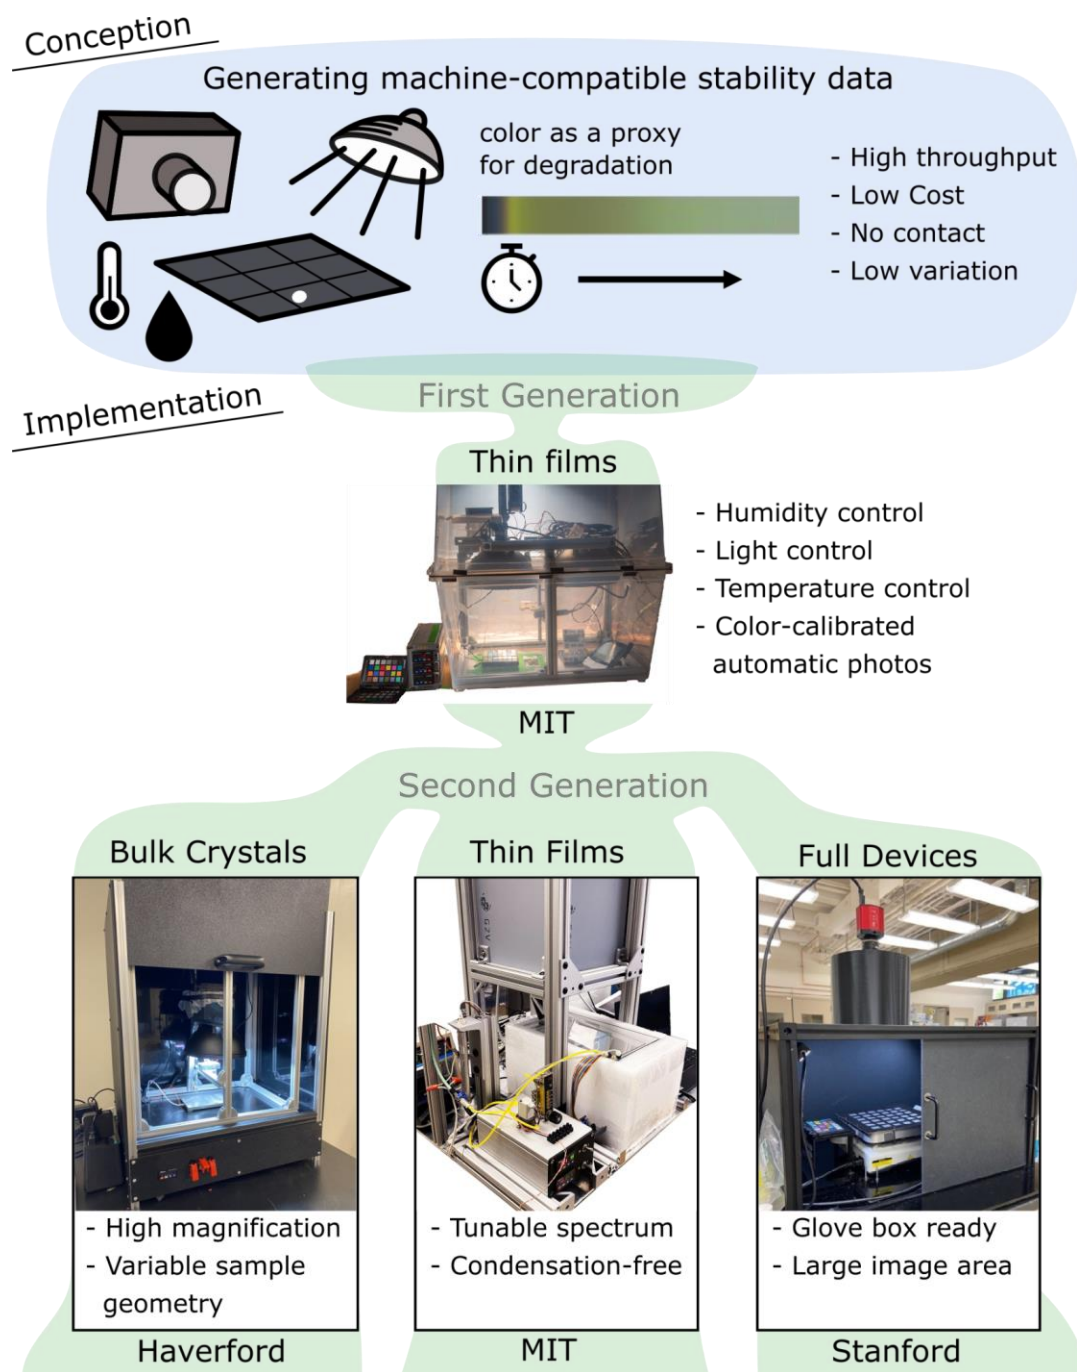


Figure 1: Environmental chamber design and evolution.

Because spectroscopy is a widely accepted method in kinetics experimentation, we propose that optical changes in the visible light spectra can be a viable substitute when samples must be observed noninvasively *in-situ* especially for materials like lead halide perovskites which have degradation pathways in the visible spectrum. Color change is often used in chemical experimentation as an indication of reactivity. In food science, automated color change analysis has been instrumental in quality assessment and sorting [25]–[27]. General chemistry pedagogical experimentation with kinetics in acid and base reactions lean heavily upon color change indicators

[28], and more machine-driven versions using smartphone cameras have since automated the analysis of optical changes to determine rate law parameters [29].

Color extends beyond a qualitative measure and can also be compared between laboratories when it is properly calibrated to account for the effects of illumination conditions and camera devices [30]. Methods such as 3-dimensional thin plate spline or root-polynomial regression are applied to convert the colors seen by the camera to the colors they would look like under a standardized reference illuminant using a reference color chart as a basis for the transformation [31], [32]. Calibrated color has been previously introduced as a quantitative metric to evaluate dye solar cell degradation [33], [34] and is used especially in color analysis applications that involve multiple devices or sites. Furthermore, calibrated color is useful when small-area colorimeters are not sufficient due to the spatial variability of the samples such as in the food industry [25], [27], [35].

We hypothesize that materials properties of interest such as electronic structure, composition, and defects have optical signatures, which can be rapidly measured and correlated with high-fidelity structural or electronic characterization methods. This is not a bidirectional relationship; while the presence of color change indicates some mechanism of material decomposition, the lack of color change does not imply stability. An optical proxy is thus a strong but noncomprehensive indication of material instability. This approach can be applied to perovskite degradation because halide perovskites like methylammonium lead iodide (MAPbI_3) undergo phase transitions with distinct colors during degradation. By examining color change, we argue that it is possible to non-invasively monitor degradation kinetics in longitudinal perovskite testing.

2b. Color as a proxy for perovskite degradation

In this section, we present the optical proxy for perovskite stability based on the change of color. We establish correlations between perovskite color change and (1) solar cell device degradation for thin-film samples, and (2) changes in X-ray diffraction (XRD) patterns for bulk crystals. A combination of earlier results from the authors and new analyses is shown.

To establish trust in an optical measurement as a proxy for phase change, the limits within which optical proxies are valid are analyzed and possible false relationships identified. As the authors did not have access to an *in-situ* XRD tool, we established the following correlations: (1) For ensembles of samples, we compared centroids of pre-degradation XRD data with the centroids of the time-resolved RGB-camera-based measurements, using clustering methods to identify centroids (Figure 3). (2) For individual samples, we measured XRD before and after degradation, and compared to color changes (Figure 4). We also reference a prior study that examines changes in perovskite RGB color change with solar-cell device efficiency, shown in Supplemental Information Figure S1. The limits of this color-based proxy are explored in the last paragraph of this sub-section.

Evidence for MAPbI_3 perovskite film color serving as an indicator of perovskite solar cell degradation was directly established in Hashmi *et al.* [36]. Evidence for correlation between the color and efficiency change is shown in Figure 2a, with color change of the solar cells in Hashmi *et al.* shown as a function of their efficiency. Efficiency values in Figure 2a are linearly interpolated due to the different time points of measuring efficiencies and colors, see Supplementary Section

S1). Color works as a proxy here, because one of the perovskite decomposition products, PbI_2 , has a much larger bandgap (2.27 eV [37]) than the original film, MAPbI_3 (1.52 eV [38]). This results in the yellowing of lead iodide perovskites under environmental stress. The utility of the color proxy as a means to identify more stable perovskite compositions was demonstrated in a study by Sun, Tiihonen *et al.* [39] as shown in Figure 2b: Proxy measurements on bare films within the MA-FA-Cs lead iodide quasi ternary phase diagram — implemented using the first generation degradation chamber shown in Figure 1 — indicated a more stable composition centered at $\text{Cs}_{0.17}\text{MA}_{0.03}\text{FA}_{0.80}\text{PbI}_3$; it was 3x more stable than the reference state-of-the-art $\text{Cs}_{0.05}(\text{MA}_{0.17}\text{FA}_{0.83})_{0.95}\text{Pb}(\text{I}_{0.83}\text{Br}_{0.17})_3$ and yielded in 30% less degradation in a damp heat test when tested directly at the device level.

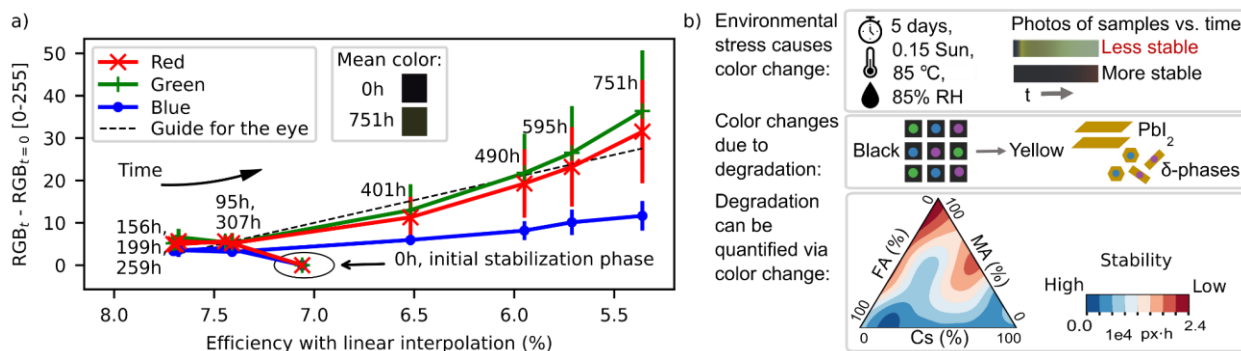


Figure 2. (a) Evidence for the correlation between perovskite film color and device performance. Efficiencies and color changes were measured by Hashmi *et al.* in [36]. The colored patches represent the sample color before and after the aging test. The efficiency values shown here are linear interpolations to the time points of color measurements. (b) Color change in perovskite films can be used as a quantitative proxy for degradation, established by Sun *et al.* [39]. Data in (a) reprinted and figures in (b) reprinted and adapted upon request to Journal of Materials Chemistry A and Matter, respectively.

A correlation between color and degradation is established within the limits of the decomposition products remaining optically distinguishable from the original phase within the wavelengths defined by the equipment. Optical cameras with Red, Green, and Blue channels (approx. 550–700 nm, 450–650 nm, and 400–550 nm, respectively, for commercial cameras but highly dependent on the camera model [40]) have reduced sensitivity for colors outside their spectral sensitivity area, *i.e.*, approximately below 1.78 eV. The spectral sensitivity range of commercial cameras can be extended to up to approximately 900 nm (1.4 eV) [41] by the removal of an integrated infrared filter from the camera. The spectral sensitivity of each setup should be measured because the camera lens and other components absorbing irradiation affect the result. For example, the mixed MA-FA-Cs lead iodide perovskites investigated in Sun, Tiihonen *et al.* [39] have a potential degradation route *via* dark minority-phase formation (*e.g.*, perovskite-structured CsPbI_3 suggested with computationally estimated bandgap of 1.57 eV [42]) in addition to decomposition of perovskite into yellow by-products. Thus, the infrared filter was removed from the camera in the first generation MIT chamber (Figure 1) to better avoid these dark-coloured “false positives”.

Color could potentially be a *lagging* indicator of device efficiency because, by the time the film color has noticeably changed, the concentrations of other defects (including point defects) may already be high enough to affect device performance. The precise amount of the lag depends on

the point-defect chemistry, composition, and degradation pathways of the film. For the example shown in **Figure 2a** and Supplementary **Figure S1**, the lag is less than 142 hours over a total test time of 800 hours. The comparison of the average colors of the samples before and after the aging test (**Figure 2a**) indicates that also subtle color changes can be quantified by the color-calibrated photographing procedure. Generally, as long as the lag remains constant or has less variability than the change of degradation onset between the target and reference samples, the optical proxy remains useful.

The conception of the degradation chamber in this work aims at high-throughput, machine-interpretable degradation data that can be used to run automated searches for more stable materials. To avoid false positives when exploring unknown compositional search spaces – especially with low level of human intervention, as is often the case in high-throughput experiments – the authors recommend clustering the optical data retrospectively for targeted in-depth analysis. Here, we demonstrate the clustering approach for the perovskite film samples of varying MA-FA-Cs lead iodide compositions from Sun and Tiihonen [39]. We cluster the optical data without composition information and target the XRD analysis to the compositional and optical centroids of the clusters. The comparison illustrates that the clusters with differing color change behaviors have compositional and phase differences already as fresh samples, thus strengthening the color proxy.

Three color clusters were identified among the samples by feeding the time-series optical data (concatenated time-series of the red, green, and blue pixel values of each sample) into the hierarchical clustering algorithm (Supplementary **Figure S2**, detailed description of the approach in the Experimental). These three color clusters were then overlaid atop the quasi-ternary composition diagram, as shown in **Figure 3a**. The mean RGB color data (**Figure 3b**) shows the differing degradation fingerprints among the clusters. In RGB representation, yellowing of the perovskites (due to perovskite decomposition into PbI_2) is seen as the blue color decreasing relative to the green and red colors. Cluster 0 shows yellowing throughout the aging test, cluster 1 retains color relatively well, and cluster 2 samples retain color after the changes seen in the first minutes of the aging test, yet the stabilized color is yellow.

Two cluster centroids were chosen from each cluster; the compositional centroid and RGB centroid that is the most typical color degradation curve. XRD is analyzed from the non-aged cluster centroids (**Figure 3c-h**). All of these samples were dark and similar by the eye as fresh samples (Supplementary **Figure S2**). Nevertheless, the XRD analysis shows distinct patterns between the clusters. Both cluster 2 centroids (**Figures 3c and 3f**) show distinctive features from clusters 0 and 1 attributed to their high $\delta\text{-CsPbI}_3$ content. $\delta\text{-CsPbI}_3$ is an orthorhombic perovskite phase that is yellow and non-photoactive, and in high content it may even result in the film appearing yellow. During aging tests, this yellow phase is also an accelerator for α -perovskite degradation, possibly by acting as nucleation centers for decomposition [39]. In cluster 1 samples, more Cs are incorporated into the α -mixed-cation-perovskite, and excess PbI_2 remains in the film. Higher Cs in perovskite crystal structure in cluster 1 samples is evident by the contraction of the cubic perovskite lattices, shown in the right-shifted (001) perovskite peak at around 14° . During aging, the incorporation of Cs into α -perovskite lattice is expected to improve perovskites' thermal stability, leading to a delay in the color transition between the black α -mixed-cation-perovskite and its decomposition product of yellow PbI_2 . We shall note that the stabilization effect from Cs incorporation is counterbalanced by the accelerated degradation due to the presence of excess PbI_2 .

Finally, the XRD patterns of cluster 0 samples show combined features of the two other clusters. The increased MA content in cluster 0 compared to cluster 1 leads to weakened moisture stability during aging tests, where the films are expected to turn from black to light yellow till transparent under high humidity. Cluster 0 also has increased δ -CsPbI₃ content compared to cluster 1.

Based on the XRD of the freshly measured cluster centroids, both RGB and compositional centroids within each cluster show same type of XRD patterns, and differing XRD patterns between the clusters, which is expected to lead to stability differences: Cluster 1 > Cluster 0 > Cluster 2. This is in line with the observations from the RGB data. The XRD analysis of the cluster centroids helps in this case also revealing and explaining a potential source of false positives in the examined compositional region, because cluster 2 compositions with high content of non-photoactive δ -CsPbI₃ are not likely to result in high-performing solar cells. This example illustrates that the spot-checks of cluster centroid samples serve as an effective route to understanding the main features of the investigated material domain when it is not desirable to expose all the samples to extended characterization.

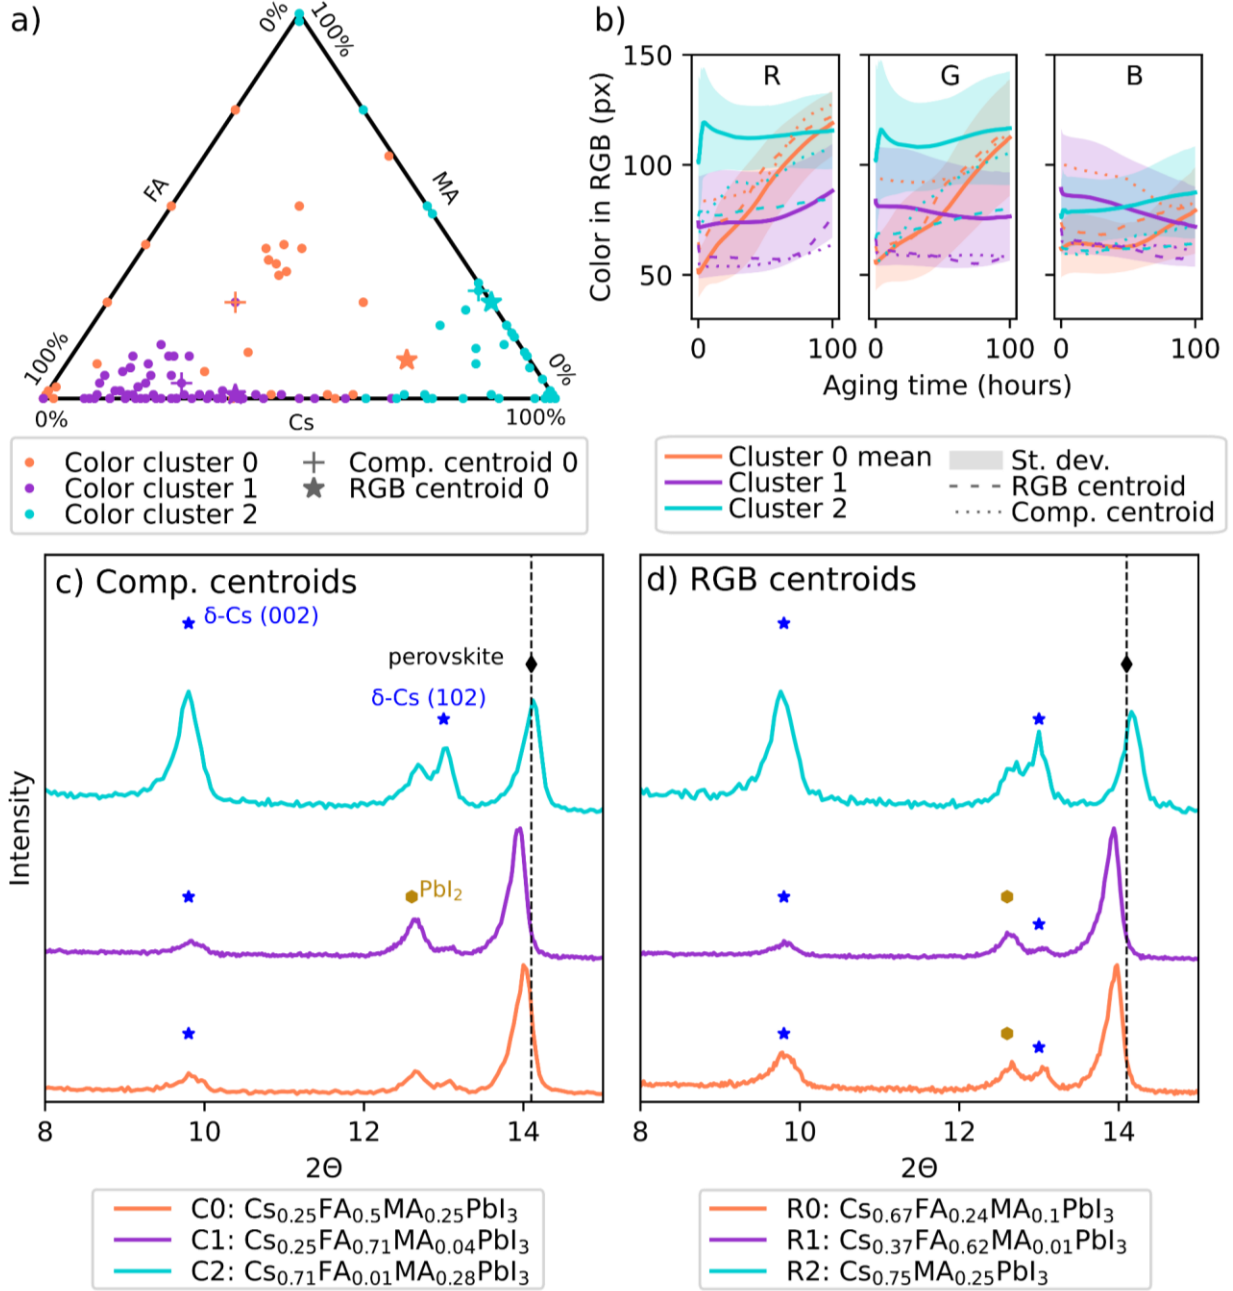


Figure 3. In-depth analysis of perovskite samples can be targeted by clustering the color degradation data (shown here for $\text{Cs}_x\text{MA}_y\text{FA}_{1-x-y}\text{PbI}_3$ film samples degraded under heat, humidity, and illumination stress by Sun et al. in [39]). Three clusters are identified from the color data by hierarchical clustering with cosine distance metric. a) The three color clusters show compositional differences when the clusters are overlaid to the composition domain. Each dot is a perovskite sample. Individual samples that are located nearest to the cluster centroids in terms of composition (crosses) and the most typical RGB degradation data (asterisks) are highlighted. (b) Mean RGB color degradation data with standard deviation shown for each cluster. The individual compositional and RGB centroid data are highlighted. X-ray diffraction patterns of the (c) compositional centroid (C0-C2 for clusters 0-2, respectively) and (d) RGB centroid (R0-R2)

samples. Blue stars label δ -CsPbI₃, yellow hexagons PbI₂, and black diamonds α -mixed-cation perovskite phase.

Next, the color proxy is extended to bulk samples in addition to perovskite film samples. In this case, device efficiency is not a direct usable metric, therefore changes in crystal structure are used to elucidate the extent of degradation. Powder XRD analysis was performed before and after longitudinal aging tests. Samples were aged for 150 hours at 0.15 Sun, 85°C and 85% RH. As with thin film testing, image capture was performed at the visible wavelengths, with analysis of RGB channels.

Bulk crystals have a smaller surface-area-to-volume ratio than thin films. This means that degradation observed via optical change occurs at the surface of the sample but may not be indicative of subsurface structural change when the crystals are opaque. To address this limitation, crystals were ground and spread thinly across filter paper sample holders to ensure uniform degradation across the volume of the samples and increase the kinetics of degradation.

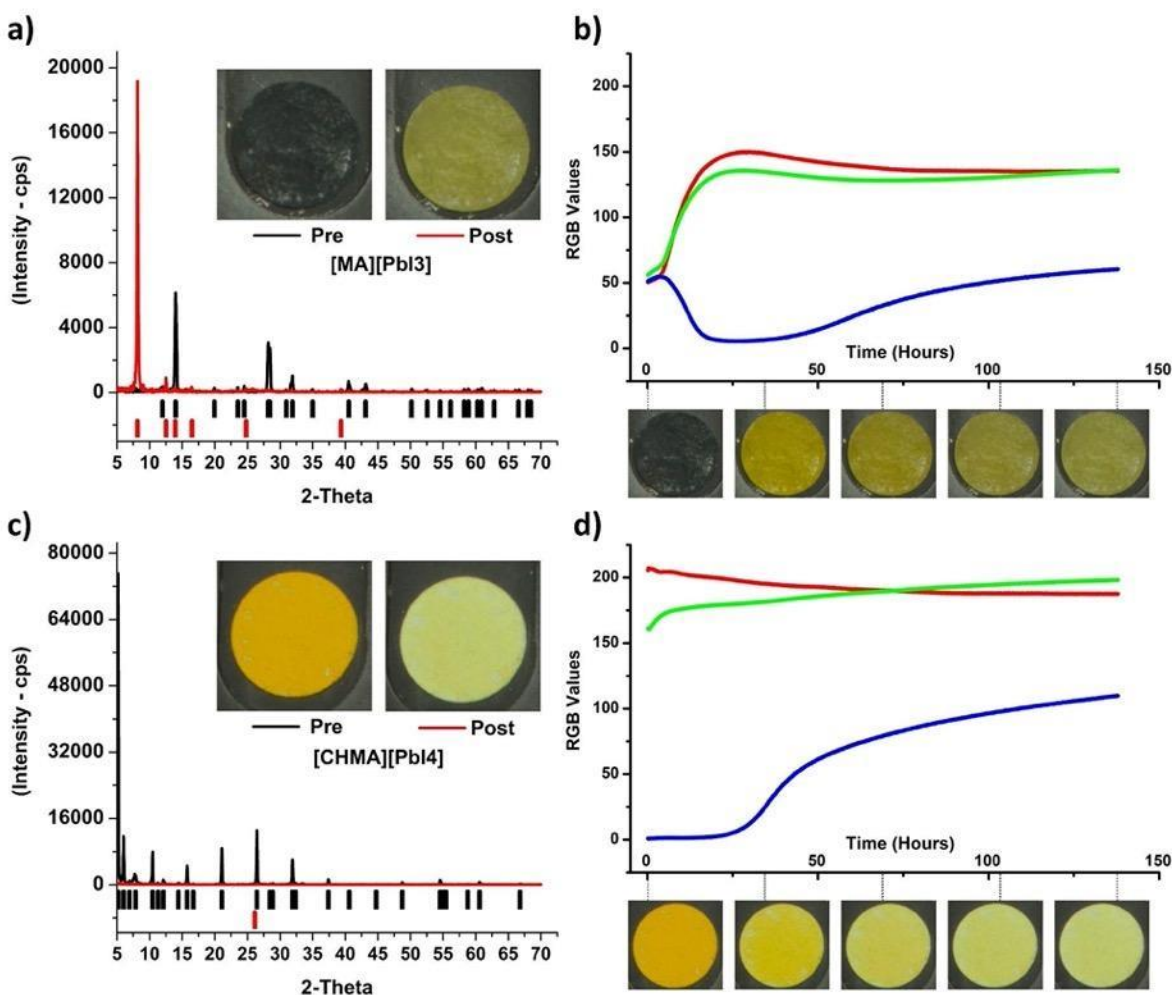


Figure 4. (a, b) Pre/post powder XRD patterns and color change time-series for MAPbI₃, and (c, d) [CHMA][PbI₄] bulk samples.

The complete reduction in peak intensity in the [CHMA][PbI₄] crystals (**Figure 4c**) shows that Bragg's Law no longer holds; the samples are no longer crystalline after the degradation test. In the MAPbI₃ samples, the shifts in peak intensity illustrate the change to another crystalline structure (**Figure 4a**).

In summary, color change is established as a reliable proxy for degradation in perovskite bulk samples, thin films and solar cell devices, and has aided researchers to improve perovskite device stability. This proxy is valid within the following limits: (1) the decomposition phases are optically distinguishable from the original film at the wavelengths selected for the hardware (light source and imaging system), (2) the lag between color change and device efficiency decrease is sufficiently small, and (3) bulk samples have a sufficiently large surface area to volume ratio such that surface degradation is representative of overall degradation.

3. Implementations

3a. First generation chamber at MIT (thin films)

The MIT Environmental Chamber Gen. 1 (Figure 5) is designed for high-throughput degradation testing of perovskite films with areas of approximately $1.27 \times 2.54 \text{ cm}^2$. Color change is used as a proxy for degradation which is induced by environmental stress from the heated sample holder (up to 100 °C), increased air humidity (up to approximately relative 85% air humidity depending on the level of heating), and illumination (up to 0.16 Sun visible light). Calibration data for the chamber is available in the open access documentation repository supplementing this article (see Data and Code Availability statement). The chamber is easily expandable for higher-throughput testing. It can fit 28 thin film samples under each camera-lamp pair and at maximum two pairs of lamps fit into the chamber. The components are chosen primarily so that they are widely and readily available with reasonable cost, and can be adapted apart from the main parts (the lamp, camera, lens, and reference color chart shown in Figure 5). Therefore, this version of the chamber serves as a straightforward path for implementing automated aging testing capacity for any laboratory willing to expand towards stability research. The cost range of this version of the chamber is US\$2,000-\$5,000 depending on the amount of reused materials utilized in the process.

The structure of the main parts within the chamber is illustrated in Figure 6a (detailed description in the documentation repository, see Data and Code Availability statement). The humidity of the chamber is controlled via an Arduino-driven stand-alone software (shared in the code repository, see Data and Code Availability statement). The sample holder temperature is controlled with a resistive heater - thermocouple pair. The chosen LED lamp is stable enough to be used with a fixed operation voltage during aging tests with durations from days to few weeks. In addition to the controls, the chamber includes a separate high accuracy air temperature and humidity logger as well as a feature for detecting possible lamp failures or lamp aging retrospectively from the image data (described in the documentation repository). The building block design presented above facilitates implementing only the necessary parts of the chamber when the design is adapted for future applications.

The sample holder (Figure 6b) is made of graphite to conduct heat efficiently and is painted with matte, neutral gray paint to avoid interfering with sample photography. Pins are used for mounting the samples accurately on the sample holder, and the surfaces are tilted to reduce specular reflectance of the perovskite film samples. The sample degradation during the aging test is monitored via a ThorLabs DCC1645C CMOS camera that is attached to the lamp dome (Figure 6c). The camera was ordered from the manufacturer with the infrared filter removed, in order to expand the spectrum of the camera. The camera is controlled with a LabVIEW program (shared in the code repository) in which the main camera settings can be adjusted according to the illumination conditions and the frequency of taking pictures is set. Additional electric contacts can be added to the sample holder for expanded *in-situ* characterization but are opted out in this chamber version. This is because a minimum design producing data for machine learning -aided high throughput aging testing was desired, *i.e.*, the priorities were simple, expandability and data with machine-readable quality with minimal interventions.

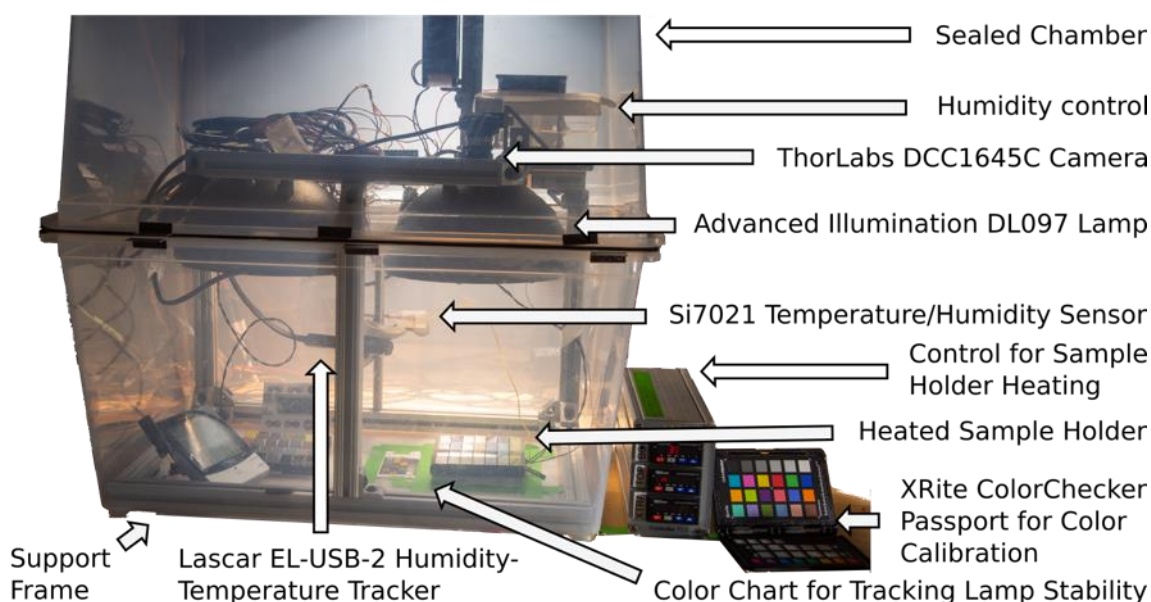


Figure 5: The MIT Aging chamber Generation One with the main components identified. Excluded from the image are a control laptop, Arduino humidity controller, and a darkening curtain that is placed on top of the chamber when the chamber is running. The LED lamp is ring-shaped and has a conical shade to produce even illumination to the 4×4 inch² sample holder area. The humidity is controlled by evaporating water with a fan, and additional fans even out the humidity and temperature across the chamber. Two lamp-camera-sample-holder combinations fit into the chamber that is sealed with an insulation band and clips.

Image data is analyzed after the aging test with a Python script (shared in the code repository). Due to the consistent shape of the samples, the script is designed to crop the images to the sample holder only, slice them to single sample sub-images, average the color over the sample, and color calibrate them (a result from the script analysis is shown in Figure 6d). The color calibration is performed by the aid of XRite ColorChecker Passport (Figure 5). It is photographed in the chamber in the place of the sample holder as the first image of each aging test, and used as a reference. The

difference between how the color of each color patch is known to appear under a D60 reference illuminant and how they are observed by the camera in the aging chamber is used as a basis for calibrating the colors of the samples. The color calibration is implemented via a 3-dimensional thin plate spline transformation from the color space of the chamber to the reference color space, first transforming the colors from RGB color space to LAB color space, then applying the spline transformation, and transforming back to LAB color space. The approach is described in detail in the Supplementary Material of our previous work [39] and the code implementation is integrated into our analysis script (shared in the code repository). The Python script applies the color calibration automatically to all but the first picture in the aging test data folder and produces graphs on the average color-calibrated sample color as a function of the aging test duration (Figure 6e).

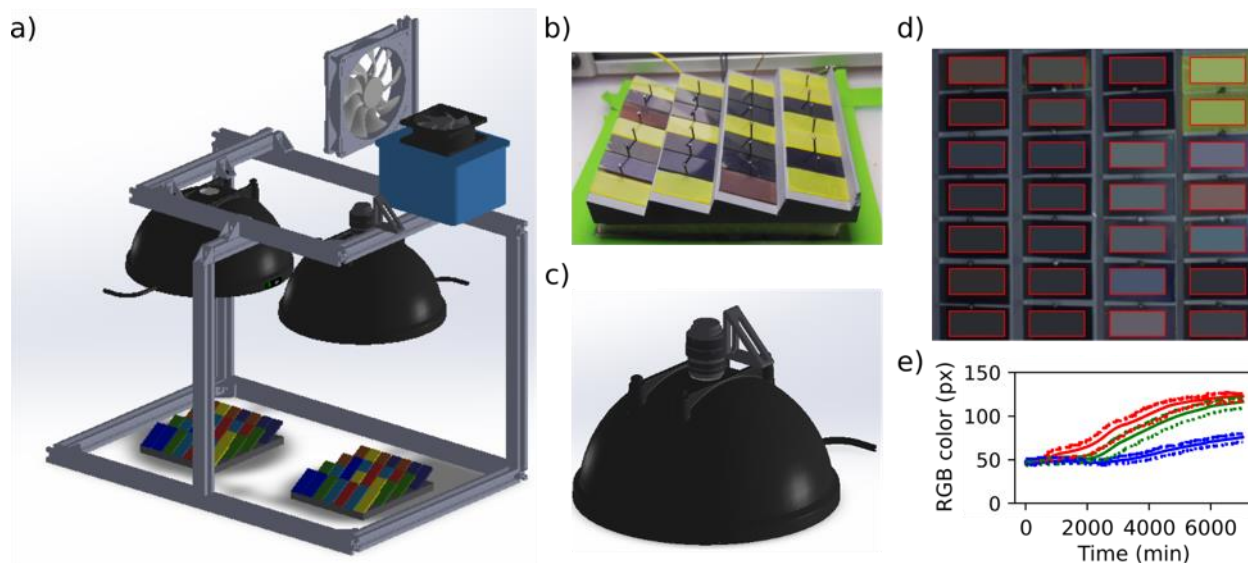


Figure 6: Construction of the MIT Generation One Chamber. (a) Support frame with lamps, cameras, and evaporative humidity control system attached. (b) Graphite sample holder loaded with high- and low-Cs content perovskite film samples. (c) The programmable camera is positioned to look at the samples through a hole in the conical shade of the lamp. (d) Python analysis script crops the image to the sample holder area, slices it to pieces containing the interior of each sample, averages the color and color calibrates it. (e) Average red, green, and blue (RGB) pixel color of an exemplary perovskite sample over the aging test duration.

3b. Second generation chamber at Haverford (bulk crystals)

The design principle of the Haverford Group's Aging Chamber (Figure 7) is to optimize image capture with bulk-crystal perovskite samples. Bulk-crystal samples have variable geometry, positioning on the substrate, and a smaller absolute, observable surface area compared to thin films. The samples in this chamber are placed in nine separate wells, allowing for the simultaneous testing of up to nine different samples. The surface area of the bulk crystal samples ranges from 0.5 – 1.5 cm². To adapt the chamber to the specific workflow and sample type, the image acquisition software was modified along with the sample heating/holding assembly, and chamber enclosure, while keeping most of the hardware choices in the first generation chamber. Minor

changes were made in terms of hardware placement, microcontroller choice, electronics storage, and data acquisition scripts to suit lab operators' preference.

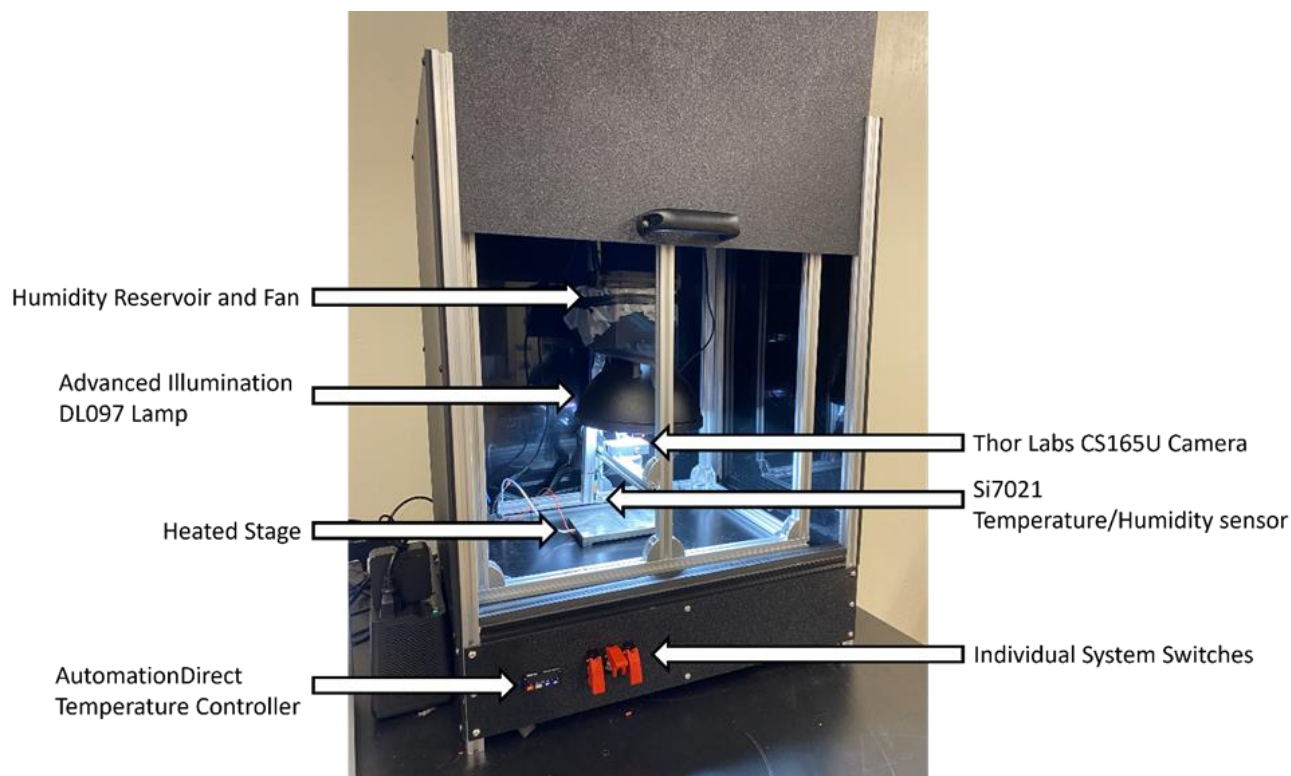


Figure 7: The Haverford Environmental Chamber, for measuring bulk crystalline samples, with key componentry labeled.

Hardware Changes:

The Haverford aging chamber uses the same lighting, image acquisition, humidity control, and heating hardware as the first generation chamber. However, image acquisition of smaller samples (necessitating a shorter focal length and higher magnification) is more sensitive to refraction from changes in ambient temperature within the chamber. As the chamber comes up to temperature, the image from the camera distorts due to the changing temperature gradient in the air. Hardware modifications were made to reduce air temperature fluctuations within the chamber. The chamber needed to be preheated to stable operating temperature before samples were loaded and to return to thermal equilibrium quickly after loading. To accomplish this, the Haverford chamber has a different enclosure **Figure 8(a)** with a vertical sliding door to reduce temperature loss when loading **Figure 8(a1)**, and a heated stage with high thermal mass **Figure 8(c4)** to minimize the temperature dip when the sample holder **Figure 8(c3)** is added.

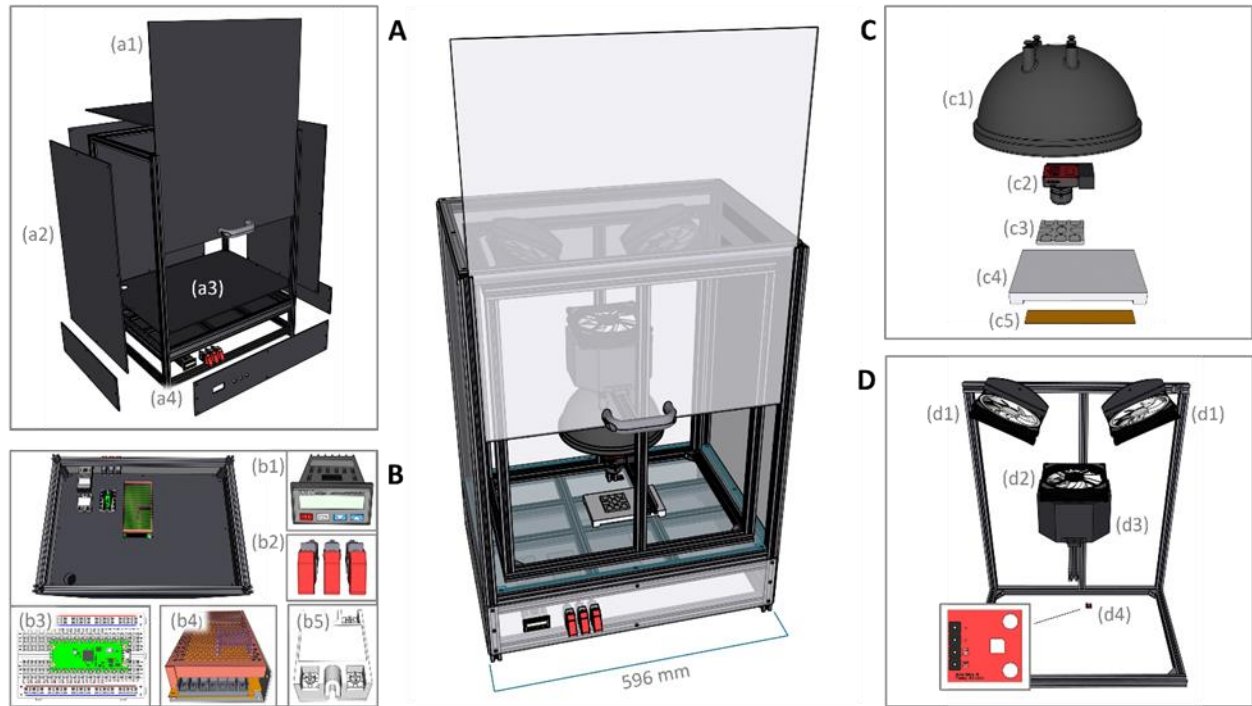


Figure 8: An overview of the Haverford Environmental Chamber, and the modified systems. (a) The chamber enclosure. (b) The electronics compartment (from bottom), and electrical components. (c) The imaging/lighting system, and the sample heating system. (d) The humidity control system.

The Haverford Chamber's enclosure **Figure 8(a)** is built from aluminum extrusions and ABS paneling **Figure 8(a2)**. The floor of the chamber is a G10 – FR4 Fiberglass-epoxy laminate panel (“Garolite”) **Figure 8(a3)** to withstand the heated stage without warping. The chamber is sealed with sealant tape compressed between the panels and the aluminum extrusions. The opacity of chamber walls eliminates the need to account for external lighting fluctuations. The underside of the enclosure contains a separate compartment **Figure 8(a4)**, **(b)** used to mount and organize the electrical components: Raspberry Pi Pico and Breadboard **Figure 8(b3)**, Power Supply **Figure 8(b4)**, AutomationDirect Temperature Controller **Figure 8(b1)**, toggle switches, **Figure 8(b2)**, and solid state relay **Figure 8(b5)**.

Modifications were made to the placement of circulation fans **Figure 8(d1)**, so that air flow to the sample stage does not shift the samples during image acquisition. The water reservoir is 3D printed **Figure 8(d3)** to mount to the chamber frame and press fit with the humidity control fan **Figure 8(d2)**. The SI702 temperature/humidity sensor **Figure 8(d4)** is mounted on an aluminum extrusion close to the heated stage. The chamber uses the same Advanced Illumination DL097 lamp **Figure 8(c1)** as the MIT Gen 1 design. The ThorLabs CS165CU camera is lowered **Figure 8(c2)** closer to the sample holder, and the focal length of the lens (ThorLabs MVL6WA) is adjusted to increase magnification. The total hardware cost for the Haverford chamber is estimated at US \$2500.

Software Changes:

Haverford Chamber uses calibrated color change in perovskite crystals as a measure of their instability. bulk crystalline samples require a new image analysis pipeline to extract degradation data because (1) they are smaller than the thin films analyzed in the first generation chamber, (2) they do not entirely fill up the sample holder, and (3) their exact locations are variable. To address this challenge, the Haverford Chamber has an automated image acquisition pipeline implemented with OpenCV in Python. This pipeline uses computer vision to automatically isolate single crystal samples from the captured images and extracts their color change in RGB values over time (Figure 9). This process is very useful for small samples, as the chamber can isolate them from the scene and mask the extraneous pixels.

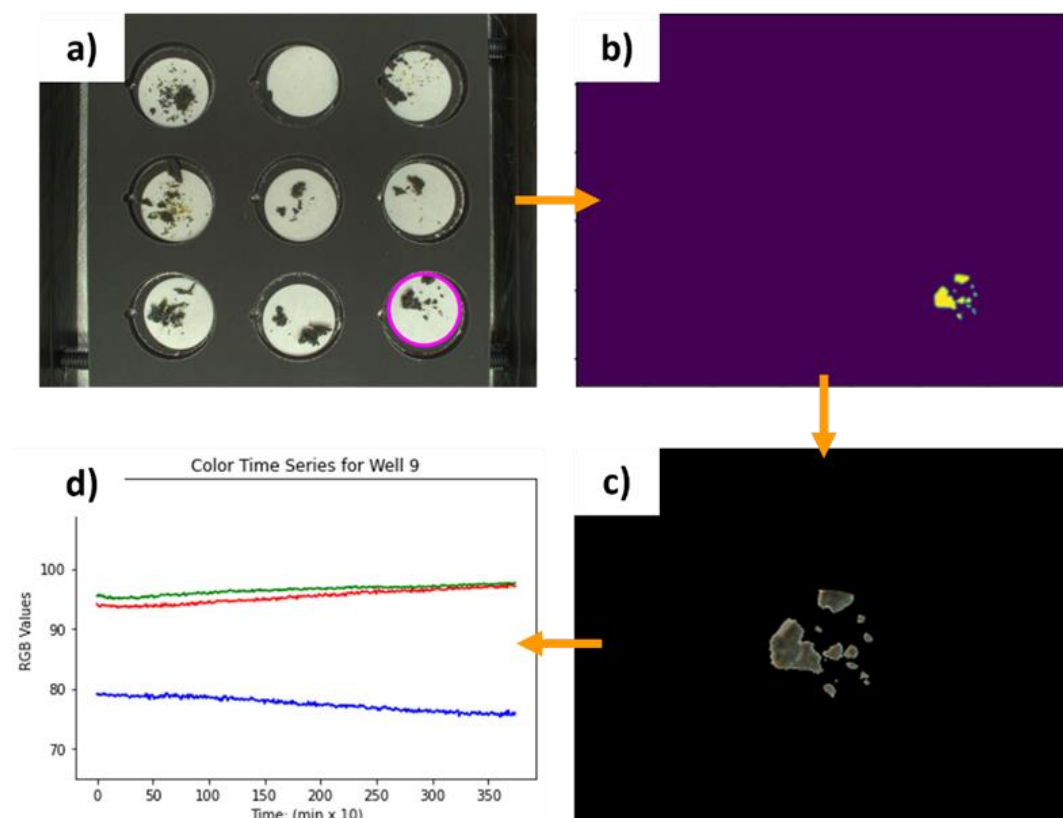


Figure 9: The image processing pipeline of the Haverford Aging chamber. (a) First, a region of interest containing the desired sample is isolated from the raw image. In this case, the samples in well 9 (bottom right corner) are selected. This is done using Hough Transform circle detection on the white filter paper underneath the samples. (b) The known color of the filter paper (acquired from a “blank” well without any samples) can be used as a greenscreen to remove all the filter paper pixels. This leaves a mask that leaves only the samples. (c) This mask is then applied over the original image. (d) The RGB values of the isolated samples can then be analyzed.

This image processing is adaptable to other samples of variable geometry. The only features the image isolation relies on are circular filter paper, and sufficient contrast between the sample and the paper. Any bulk sample that is placed on filter paper with enough contrast can be automatically isolated from the rest of the image, and its color changes extracted. This also demonstrates that

software can be treated as another submodule of the chamber and varied independently from the rest of the design for an adopter's specific use case.

To fit the scripting preferences of the Haverford operators, the original Arduino Uno was replaced with a Raspberry Pico running MicroPython. The Pico controls the humidity fan, and the two chamber circulation fans. All fans are 140 mm, powered by a 12-volt line and mounted to the aluminum frame with 3D-printed mounts. Data acquisition scripts were written in Python on the data-logging computer to compile data from the Solo 4824 Temperature Controller, the Si7021 Temperature/Humidity sensor, and the ThorLabs CS165CU Camera and save them to a specified experiment file.

3c. Second generation chamber at Stanford (full devices and modules)

The Stanford Environmental Chamber is designed specifically for imaging heat-based degradation of full solar devices as well as perovskite films produced via the rapid spray plasma processing (RSPP) method [43]. Additionally, the chamber can compare devices produced with other common fabrication techniques like spin coating with RSPP perovskite films. The chamber maintains RGB color as a means to characterize thermal degradation pathways in the perovskite thin-film solar devices similar to the first generation chamber; however, to exclude other degradation pathways, the chamber is constructed to be assembled in a glove box under nitrogen atmosphere and fully enclosed to prevent light impingement from external sources (windows, glove box lights, room lighting, *etc.*). The heat is applied directly to the films placed against a hotplate at the accelerated degradation temperature (generally 85 °C).

The Stanford perovskite films and devices encompass a variety of small cells, mini-modules, and module architectures necessitating a large imaging stage capable of fitting multiple devices simultaneously. A flat hotplate rather than the inclined substrate used in MIT's work was selected as the imaging platform to accommodate the varying perovskite films and device architectures with ease. Rather than placing the camera within the light source as is the case with the MIT Gen 1 chamber, the camera is outside the chamber to protect the electronics *via* passive cooling along with providing a large field of view. The lighting sources are placed within the box at angles to minimize glare and reflection into the lens shown in **Figure 10a**. A maximum of $36\ 2 \times 2\ \text{cm}^2$ cells and a variety of module architectures can comfortably fit on the hot plate surface as is demonstrated in **Figures 10b** and **9c**, respectively. Due to the need for a high uniformity hotplate coupled with the large field of view quality optics, the total price of the Stanford Environmental Chamber is estimated at US\$7,000. Cost reductions can easily be achieved with lower-resolution optics (from 12.3 MP to 1 MP) that still allow for quality cell imaging.

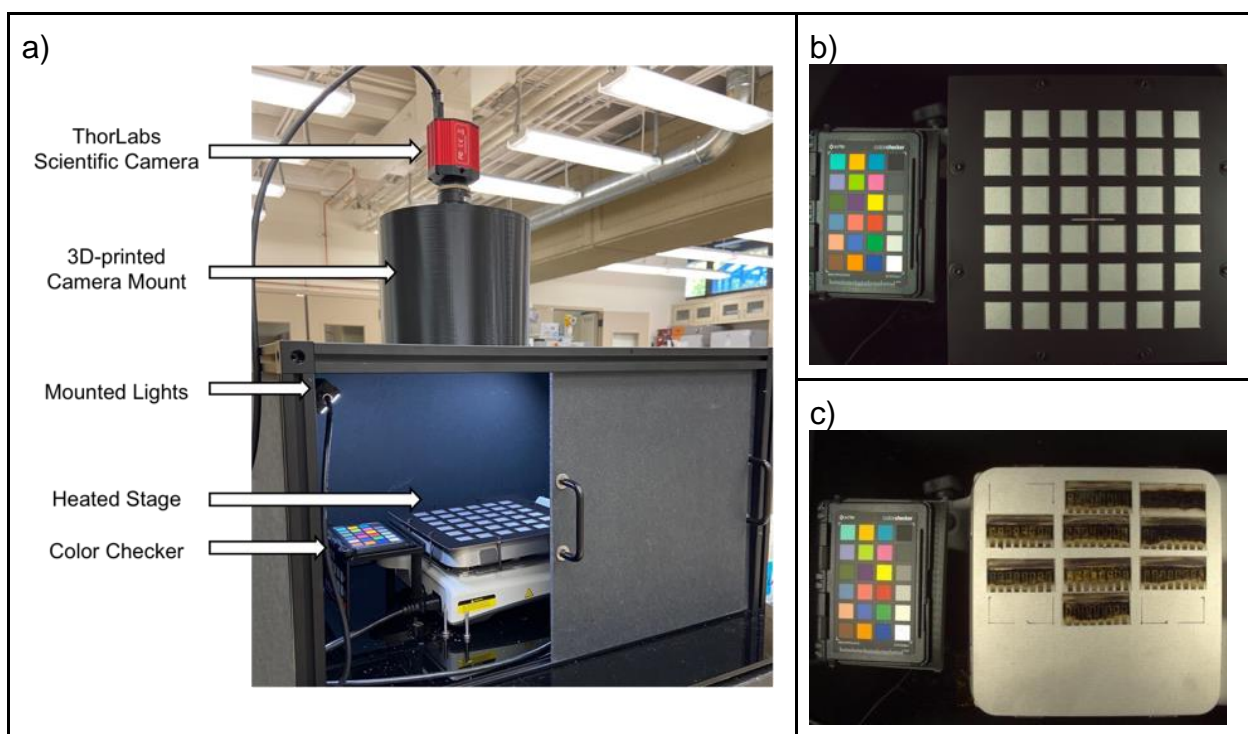


Figure 10: (a) The Stanford Enclosed Environmental Chamber composed of an illuminated and heated stage, XRite Color Checker, and mounted optical camera (ThorLabs CS126CU and MVL12M1). (b) The aligned 6×6 grid for imaging small solar cells. (c) An example of RSP module architectures on the imaging stage. The Stanford system analyzes the passport Color Checker with each image, as the system has a large illumination and imaging area of capture, allowing one to track and normalize color values against the checker along with following absolute drift in RGB values of the Color Checker between batches. Photobleaching of the Color Checker is a particular concern over thousands of hours of use and can be tracked using this approach because the checker remains in the field of view in each image. Additionally, this system can be run in two modes: continuous illumination and illumination only for photograph capture (flash mode). The two modes allow for a mitigation of device photodecay with flash mode and accelerated device photo-aging in the fully illuminated mode.

3d. Second generation chamber at MIT (thin films)

Similar to the first generation chamber, the MIT Generation 2 Chamber (Figure 11) is designed for high-throughput characterization of perovskite films and other oxygen-sensitive materials. However, the MIT Second Generation Chamber is designed specifically to have precision control of the dew point, which facilitates performing long aging tests with very high humidity levels. The chamber is integrated with a commercial solar simulator instead of an LED lamp in order to extend illumination intensity to up to 1 Sun, and to add spectral control. These features extend the chamber's capabilities for degrading durable perovskite materials and, due to 1 Sun visible illumination source, are also more compliant under consensus stability testing conditions for

perovskite solar cells [15]. This second generation chamber is designed to cost less than US\$1,500. The implementation of a commercial solar simulator for increased range and fidelity comes with an increase in chamber cost (approximately US\$7,500 with the solar simulator at the time of assembly). However, this price still remains in the low range in comparison to those of commercially available degradation chambers.

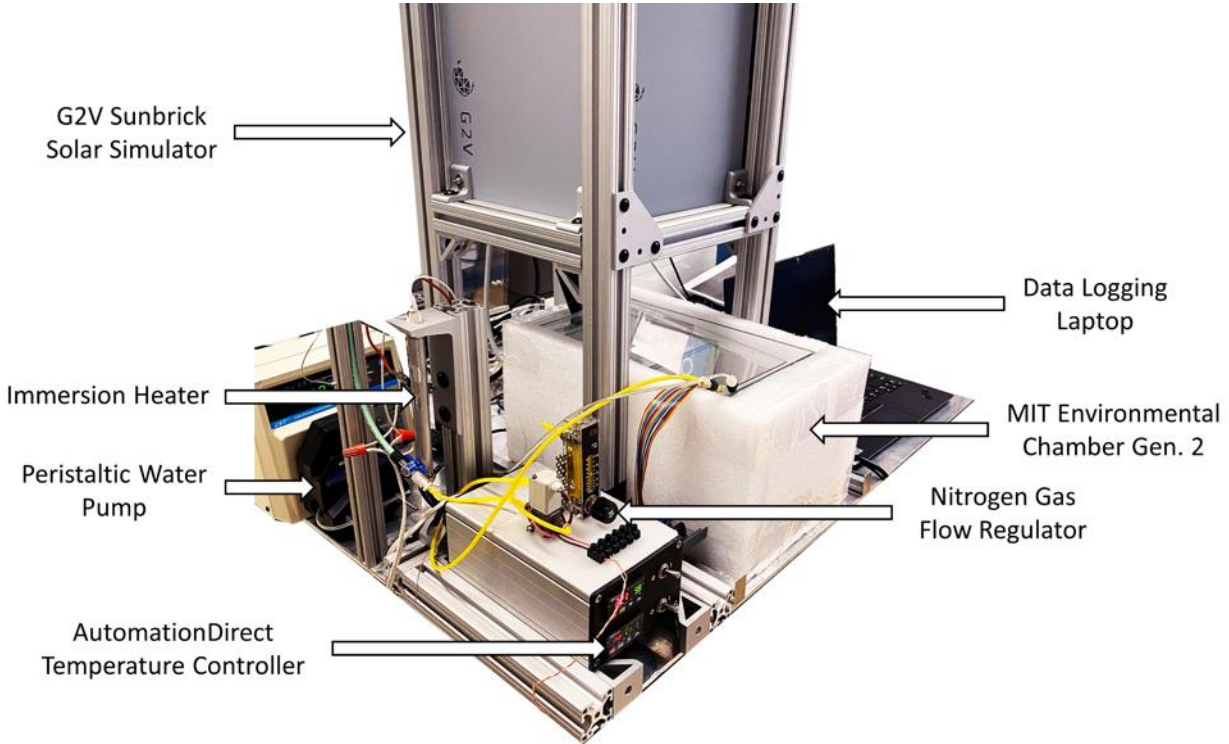


Figure 11: The MIT Environmental Chamber Gen. 2 setup. The setup for the chamber consists of an LED solar simulator, immersion water heater, peristaltic water pump, water temperature controller, nitrogen gas flow regulator, and a laptop to log data. A styrofoam casing shields the sides of the Environmental Chamber to minimize uncontrolled temperature and lighting fluctuations.

The chamber is illuminated with a G2V Sunbrick class AAA solar simulator with 625 cm² illumination area and a spectrum that is adjustable between 400-700nm. The simulator is controlled with software provided by the manufacturer. A moisture-controlled environment is attained within MIT Generation 2 Chamber through a double enclosure system where the outer enclosure is filled with water to fully submerge the inner chamber. Naturally, air within this enclosed chamber approaches its maximum saturation dew point, however, by piping dry nitrogen into the environment, the relative humidity of the air is lowered to control the dew point. Additionally, by having the chamber fully submerged in water, the temperature can be precisely controlled due to the high heat capacity of water.

The external chamber is open on the top and has a sliding lid to minimize water evaporation while the internal chamber is open on the bottom to the moisture-controlled air environment. The internal chamber is submerged into the water-filled external chamber and the upward buoyancy force is overcome by securing the internal chamber underneath a set of plastic rails, shown in **Figure 12a**.

Water is continuously circulated within the system using a peristaltic pump via a water tube, illustrated in **Figure 12b**, to both regulate the internal temperature and empty excess water from within the internal chamber air cavity. The temperature of the internal sample environment is controlled by the water temperature, which is regulated by an immersion heater and programmable controller. A dry nitrogen line runs in tandem with the water circulation line to control the relative humidity of the internal chamber by releasing dry nitrogen into the base of the internal chamber where the air cavity is located within the submerged enclosure. A base plate that holds the sample above the water line, shown at the bottom of **Figure 12c**, has a sealable door that opens when a fan, shown in **Figure 12e**, is activated to allow airflow into the chamber. The relative humidity of the sample environment is precisely controlled by tuning the flow rate of dry nitrogen into the air cavity and by circulating moist air from the water surface into the sample environment.

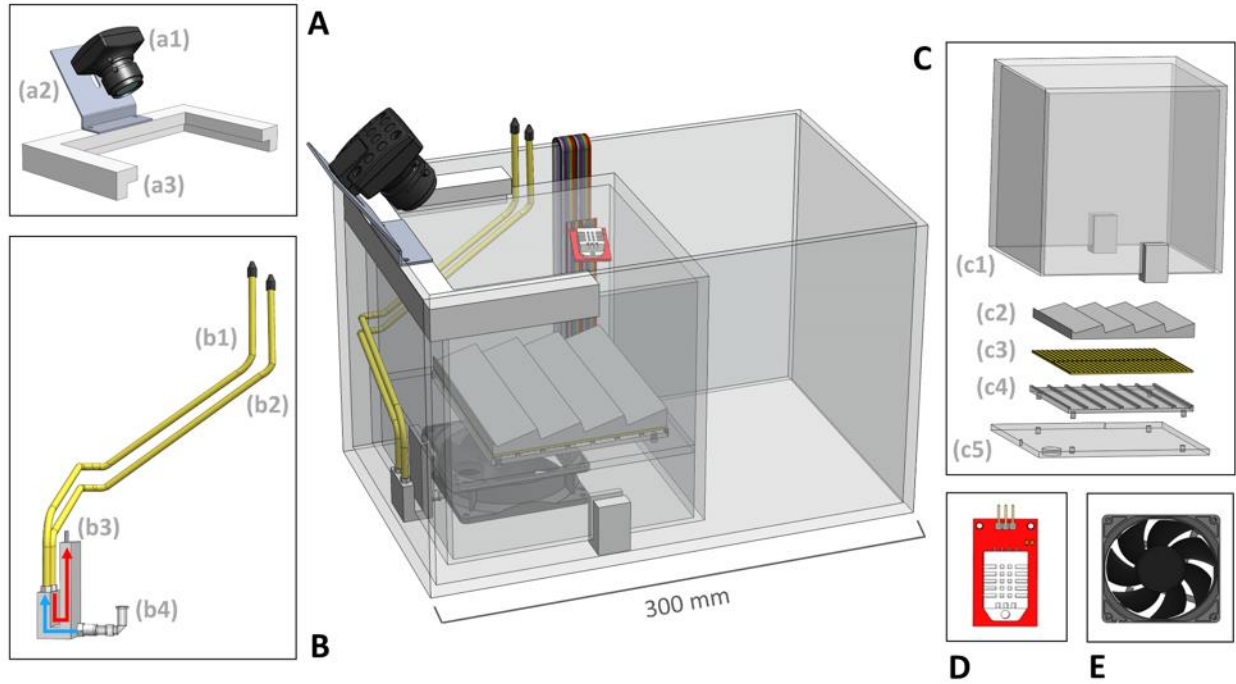


Figure 12: The MIT Environmental Chamber Gen. 2 construction. (a) (a1) A ThorLabs camera is mounted to (a2) a rail bracket for imaging the samples in a fixed position. The camera and bracket are affixed to (a3) plastic rails that push against the top of the submerged internal chamber to counteract the upward buoyancy force created by the air cavity. (b) The plumbing system consists of (b1) a water circulation line and (b2) a nitrogen gas line. Dry nitrogen gas is added to the internal environment to lower the relative humidity through (b3) the gas outlet, following the red arrow. The water level is regulated by siphoning water out of the chamber through (b4) the water inlet, following the blue line. (c) The internal chamber that is fully submerged in water consists of (c1) a five-sided enclosure with an opening at the base and plastic grippers to allow for water to freely flow under the enclosure, (c2) an angled sample holder, (c3) a thermoelectric device to heat the sample holder, (c4) an acrylic mount, and (c5) a base plate with a sealable opening that allows for air circulation within the enclosure when a fan is activated. (d) A PCB temperature and humidity sensor mounted within the internal chamber with insulated wires feeding through the base of the internal chamber and out the top of the external chamber. (e) A circulation fan used to

flow air from the moisture-controlled environment below the internal chamber into the sample environment enclosure.

Samples are mounted on the sample plate, shown in **Figure 12c**, at an angle normal to the camera line of sight. A ThorLabs DCC1645C CMOS camera (with an infrared filter removed from it) is mounted statically to a rail above the internal chamber to image the samples. A Color Checker card is placed inside the internal chamber to calibrate the camera color settings. A quartz disk is placed on the top of the chamber in the aerial transmission pathway from the samples to the camera to minimize optical aberrations due to the chamber material and water. The sample base plate has a thermoelectric module installed underneath to provide the option of directly heating the samples via conduction, as in the first generation chamber. A sensor, shown in **Figure 12d**, is mounted within the internal chamber to control the temperature and relative humidity of the internal environment. Additionally, a separate humidity-temperature tracker is used for tracking the chamber conditions, as in Gen. 1 chamber. The culminating design of the MIT Environmental Chamber Gen. 2 gives researchers better control over high-throughput materials degradation experiments in extreme humidity conditions through the precise programming of dew point, temperature, relative humidity, and illumination spectrum within the sample environment.

4. Reflections and key learnings of this open-hardware effort

The four chambers described in this work are a part of an evolutionary-design process with two distinct generations of chambers. The process provides useful insight for scientist-developers who wish to share their hardware designs efficiently yet impactfully.

This hardware disseminated and evolved organically, even accidentally. Generation 2 hardware adopters were motivated by the scientific results obtained using the Generation 1 tool, and the offer to translate the technology within the context of ongoing government-funded research projects. When developing the chamber, establishing the validity of the color change proxy was essential in encouraging hardware adoption on the other sites. In Free Open Source Hardware (FOSH) literature, this step can be likened to proof of concept and validation, where the utility of a design is firmly established, and its functionality proven [44]. In our case, the MIT team devoted the upfront cost to establish the color change proxy through prior research, which formed the foundation of the aging chamber’s experimental utility [36], [39]. While this proxy was developed in thin-film devices, the confirmed utility encouraged other sites to implement the same experimental design in other sample types. The Stanford and Haverford sites evolved the hardware toward solar-cell devices and bulk crystal samples, respectively. This expanded catalog of known use cases makes it easier for further groups to adopt the hardware in the future, and establishes a rigorous, peer-reviewed foundation for further researchers to reference, motivating the Generation 1 and 2 tool-builders to document their work.

In transferring open hardware between sites, we found that “champions” of the technology-transfer process are integral at both the “push” and “pull” sites. These key figures facilitate the knowledge transfer, and actively communicate to modify the technology for the pull site’s successful adoption. Even with thorough documentation, motivated contact persons at each site greatly facilitate implementing new use cases. At the “push” site, the champion acts to disseminate information on

the build process, direct adopters to the relevant source material, and answer any remaining questions. At the “pull” site, the champion leads the effort in sourcing, building, and modifying the hardware for the specific application. While there is significant upfront cost involved at the pull site with transferring and adopting technology, user development has been recognized by other proponents of free open source hardware as a key advantage over traditional hardware by ensuring proper functionality for specific use cases [45]. Generally, we found that funded collaborations are more successful at technology transfer than unfunded collaborations.

During technology transfer, a regular line of communication between all the active sites was essential to avoid duplication of effort, and to expedite adoption. The contact at the “push” site can nurture parallel collaboration between “pull” sites. As an example, the aging chamber’s enclosure at Haverford was replicated from observations of the Stanford group’s design. The improved enclosure increased the rate of preheating and decreased heat loss from sample loading. These types of improvements would have been more commonplace had there been an organized community of adopters who would expand the library of use cases for open hardware and act as another source of information [46]. Such a community is common-place in developer and maker culture and would reduce the burden of the push sites to support multiple adopting labs [47], [48]. In moving to share hardware with larger groups, we emphasize that an active community can crowd-source the time cost of supporting open hardware.

Resistance to knowledge drain from moving researchers is integral to ensuring longevity. A common flaw of purpose built laboratory equipment is that the knowledge to operate, maintain, and assemble the devices resides with the researchers that develop them. In academic settings, this issue is compounded by the movement of researchers to other institutions. We found that in a large project like this, knowledge is decentralized across multiple individuals. While decentralization is a major asset of open hardware [49], we found that it can provide a share of difficulty. The process of tracking down knowledgeable parties further complicates adoption by other sites. The knowledge drain and decentralization can be combated by a robust repository for all supporting files and documentation — even the beta phase documents. Storage in shared drives can be a liability; shared drive transferring issues and managing permission adds unnecessary complications with transferring between researchers and with dissemination. Even if a project begins organically with files stored internally, it is worth investing time in a robust, easily accessible file storage system like GitHub [50]. Community repositories not only allow the easy sharing of hardware assets and operational knowledge, but also motivate the push and pull site champions by providing a formal route for referring to their work, and leverage the combined knowledge of multiple adopters. Multi-modal information transfer, including videos and photos, helped improve efficiency and accuracy of communication. Of course, having a lab manager or research staff involved further supports knowledge permanence.

Thorough documentation is the most important aspect for knowledge transfer and forms the backbone of adoption. The minimum viable package in our experience includes a comprehensive bill of materials, a library of standardized file types for 3D models, a thoroughly commented codebase, manual, and a permanent repository. It will be the first point of contact that pull sites will use, and will mitigate the effort needed at push sites to support other groups. For potential adopters, a thoroughly documented repository inspires confidence that the open source hardware is well supported, maintained, and achievable to build. To that end, to foster dissemination,

hardware design should assume the lowest common denominator in mechanical experience and machine shop support at adopters’ sites. This experience is in keeping with other established design philosophies of open hardware [44]. Using aluminum extrusions and other readily available pre-fabricated parts minimized the necessity for custom hardware and machining in this work. The use of consumer level electronics, like those available from Adafruit and Sparkfun both lowers cost, and reduces reliance on proprietary software [51], [52].

Facilitating hardware evolution allows cumulative improvements and branched applications that the initial developers could not anticipate. While it is likely beneficial to maintain a base version of the hardware like in a typical open-source code repository, in this work, we observed an added benefit from the branches that may evolve far from the baseline design and cannot be readily merged with it. From this viewpoint, creating simple community standards for documenting and sharing the work is more essential than investing on standards for adding features to the baseline design. In some cases, the latter approach can actually be prohibitive for the evolution process. The evolution can be further facilitated by thorough documentation, and open communication between sites on the strengths and weaknesses of the existing design.

5. Conclusions

We detailed the development and evolution of a stability chamber that uses color change as a proxy for degradation, to create a semi-automated system to test perovskite performance under heat, illumination, and humidity. The specific aim was to generate machine-interpretable data in a high-throughput and low-cost manner. To achieve the target, we established color change as a proxy for structural perovskite degradation in thin films. It correlates with changes in device performance arising from perovskite degradation. We also established it as a valid proxy for structural change in bulk perovskite samples, confirmed by powder XRD. The first generation stability chamber was conceived at MIT, and developed into an open source platform that underwent further evolution at Haverford, Stanford, and MIT. At Haverford, the chamber was modified to work with small quantities of bulk crystals. At Stanford, the chamber was adapted to test full solar devices in a glove box. At MIT, the chamber was adapted with expanded dew point and spectral control.

In our reflection on the open hardware-development process and laboratory adoption, we found that an open source hardware platform dramatically reduces upfront time to develop bespoke equipment. The process of inter-lab transfer, and open source dissemination is improved through dedicated individuals at both push and pull sites, thorough documentation, and open lines of communication. Not only does this increase the rate at which new labs can get open hardware running, but it facilitates the process of hardware evolution, increasing the capabilities of the platform.

6. Experimental

6a. X-ray diffraction measurements and aging tests for thin film perovskite samples

The perovskite film data used in this work for clustering analysis is originally published in [39] with full descriptions of the sample preparation and measurement processes. A condensed

description is provided here in parts that are relevant for the clustering analysis. The perovskite thin films analyzed in this work were spin-coated on cleaned and UV-ozone-treated glass substrates. Over-stoichiometric PbI_2 was used for synthesizing all the films in a molar ratio of 1.09 (PbI_2) to 1 (CsI, MAI, and FAI). Lead(II) iodide solution was prepared in 9:1 N,N-dimethylformamide to dimethyl sulfoxide solvent. The precursor solutions were mixed to their nominal Cs-FA-MA compositions, chlorobenzene antisolvent was used in the spin-coating, and the spin-coated films were annealed at 403 K for 20 min before cooling them down to room temperature, cutting them in halves, and transporting the other half to XRD measurements and the other half to the degradation test. Grazing incidence X-ray diffraction with incidence angle of 1° was performed with Rigaku Smartlab with Cu-Kalpha sources. Reference XRD spectra obtained from literature for delta- CsPbI_3 [53], delta- FAPbI_3 [54], and alpha-perovskite [39] were used as the basis of the XRD analysis of the cluster centroids. It should be noted that the thin film samples have lattice strain leading to peak shifts in the spectra compared to the reference powder samples. The degradation tests for the films were performed under $85 \pm 2^\circ\text{C}$ sample holder temperature, $85 \pm 5\%$ air humidity, and 0.15 ± 0.01 Sun visible light only illumination for 7,000 minutes using the first generation degradation chamber presented in this work. During this time, the samples were photographed automatically with 5-minute intervals. In total 168 films with varying compositions were prepared (some with duplicate compositions).

For hierarchical clustering, one perovskite film was dropped from the analysis due to its poor quality and 5 reference samples with Br content (detected in by the clustering algorithm as their own cluster) were dropped from the analysis as the purpose was to focus on iodide-only samples. The color-calibrated film color as a function of aging test duration data were clustered using hierarchical clustering algorithm [55]. Cluster distances were determined using UPGMA algorithm and cosine distance measure was used. In the resulting dendrogram, three distinct clusters were detected. Samples nearest to the compositional cluster centroids and the RGB centroids, *i.e.*, the most typical color degradation curve in the cluster, were determined for the analysis. Hierarchical clustering was chosen among the clustering algorithms due to the graphical analysis of the ideal number of clusters, which is ideal for future use of the degradation data clustering repository in repeated retrospective analysis of the degradation test data.

6b. X-ray diffraction measurements and aging tests for bulk crystal perovskite samples

The perovskite bulk sample data used in this work was created in a workflow modified to make ground samples for degradation analysis. The perovskite crystals were synthesized using bench scale antisolvent vapor diffusion. The two bulk crystal samples were prepared from stock solutions of methylammonium and lead(II) iodide dissolved in gamma-Butyrolactone, and cyclohexylmethylammonium and lead(II) iodide dissolved in gamma-Butyrolactone. The crystals were grown over the course of 48 hours, then filtered and dried. Powder X-ray diffraction measurements were performed on a Rigaku MiniFlex X-ray diffractometer using $\text{CuK}\alpha$ radiation (1.5418 \AA). Rigaku Smartlab was used to confirm the correct sample identity, reference XRD spectra were obtained from literature for $[\text{CH}_3\text{NH}_3][\text{PbI}_4]$ [56], and for MAPbI_3 [57]. The remaining sample was preserved in a vacuum desiccator until aging chamber longitudinal testing. Longitudinal testing was started less than 48 hours after sample synthesis. Samples were manually ground by mortar and pestle to a fine powder. Powder X-ray diffraction measurements were taken

one more time, to both ensure that degradation had not occurred, and to provide a pre-degradation powder pattern.

To prepare the bulk samples for degradation testing, the powder was finely spread across 10mm filter paper to enable uniform degradation across the sample and increase kinetics. Each different compound was plated in triplicate to ensure enough yield for post-degradation powder X-ray diffraction. Once loaded in the chamber, samples were held at 0.15 ± 0.01 Sol, under $85 \pm 2^\circ\text{C}$ sample tray temperature, and $85 \pm 5\%$ air humidity for ~ 150 hours. Samples in the chamber were imaged every minute. After the degradation testing concluded, the samples were removed from the chamber and post powder X-ray diffraction measurements were taken.

Data and Code Availability

Figures 3 and 4 as well as Supplementary Material Figures S2-S4 in this article contain new, unpublished analyses. The data in Figure 4 and Supplementary Material Figure S4 are available on Figshare. The data in Figure 3 and Supplementary Material Figure S2-S3 have been made publicly available by the authors in an earlier work [39] and are now exposed to clustering analysis. The aging test images and metadata are available on Figshare due to their large file sizes:

https://figshare.com/articles/dataset/MA_CHMA_pXRD_Peaks_Pre_Post/20407794
https://figshare.com/articles/dataset/MA_CHMA_System_Pre_Post_pXRD_xls/20407758
https://figshare.com/articles/dataset/Haverford_Aging_Chamber_Output_For_MA_CHMA_Pero_vskite_System/20407761
<https://doi.org/10.6084/m9.figshare/20506857>
<https://doi.org/10.6084/m9.figshare.20523327>
<https://doi.org/10.6084/m9.figshare.20521173>

The aging test image data rendered into a widely usable form (*i.e.*, csv files with raw and color-calibrated color as a function of time for each sample and metadata files with sample compositions) and XRD data, as well as the analysis codes directly reproducing Figure 3 and Supplementary Material Figure S2 are shared in an open repository:

<https://github.com/PV-Lab/cluster-perovskite-data>

All the documentation, CAD drawings, control and analysis codes, and calibration data of the four degradation chambers presented in this work are shared in the following open repositories.

MIT Gen. 1 build and analysis of the image data (version used for this work is 1.0):

https://github.com/PV-Lab/hte_degradation_chamber
<https://github.com/PV-Lab/RGBanalysis>

Haverford Gen. 2 build and analysis of the image data (version used for this work is Haverford_1.0):

https://github.com/rodolfokeesey/Haverford_Environmental_Chamber

Stanford Gen. 2 build and analysis of the image data (version used for this work is Stanford_1.0):

<https://github.com/ThomasWColburn/Stanford-Environmental-Chamber>

MIT Gen. 2 build (control and analysis with MIT Gen. 1 codes):
https://github.com/PV-Lab/hte_degradation_chamber_gen2

Author Contributions

Authors R.K., A.T., C.B., A.E., and S.T. wrote codes for the chamber use and data analysis; R.K., A.T., T.C., J.S., M.Z., K.H., C.G., A.E., and Z.L. built the equipment; R.K., A.T., A.S., T.C., S.S., N.H., Z.L., F.O., J.T., A.N., and T.B. conceived of and executed the experiments; and A.T., R.D., A.N., and T.B. conceptualized and supervised the research. Authors R.K., A.T., A.S., A.N., and T.B. wrote the first version of the manuscript. All the authors participated in planning of the work and reviewing and editing the manuscript.

Acknowledgements

The authors thank Antonio Buscemi and Isaac Metcalf for assistance in XRD measurements, and Shreyaa Raghavan for the development of the user-friendly Python package. This study is based upon work supported by the Defense Advanced Research Projects Agency (DARPA) under contract no. HR001118C0036. Any opinions, findings and conclusions or recommendations expressed in this material are those of the authors and do not necessarily reflect the views of DARPA. S.S., N.T.P.H., A.T., and T.B. thank TOTAL S.A.. The research is also supported by Singapore Massachusetts Institute of Technology (MIT) Alliance for Research and Technology's Low Energy Electronic Systems research program. A.T. was supported by the Academy of Finland (Flagship program: Finnish Center for Artificial Intelligence FCAI). F.O. was supported by the U.S. Department of Energy under Photovoltaic Research and Development program under award DE-EE0007535. T.W.C. acknowledges the support from the Graduate Research Fellowship Program (award no. DGE-656518) from the U.S. National Science Foundation.

Conflict of Interest Declaration

Two of the authors (ZL, TB) own equity in a startup company, Xinterra Pte. Ltd., which applies machine learning to accelerate materials development. One of the authors (AJN) is a scientific advisor to Atinary, which applies machine learning to accelerate materials development. We open sourced all information in this study to ensure that all benefit equally.

References:

- [1] Y. Fu, J. Li, H. Luo, C. Du, and X. Li, "Recent advances on environmental corrosion behavior and mechanism of high-entropy alloys," *J. Mater. Sci. Technol.*, vol. 80, pp. 217–233, Jul. 2021, doi: 10.1016/j.jmst.2020.11.044.
- [2] N. Birbilis, S. Choudhary, J. R. Scully, and M. L. Taheri, "A perspective on corrosion of multi-principal element alloys," *Npj Mater. Degrad.*, vol. 5, no. 1, Art. no. 1, Apr. 2021, doi: 10.1038/s41529-021-00163-8.
- [3] Y. Luo, K. Song, X. Ding, and X. Wu, "Environmental sustainability of textiles and apparel: A

- review of evaluation methods,” *Environ. Impact Assess. Rev.*, vol. 86, p. 106497, Jan. 2021, doi: 10.1016/j.eiar.2020.106497.
- [4] J.-M. Kim, X. Zhang, J.-G. Zhang, A. Manthiram, Y. S. Meng, and W. Xu, “A review on the stability and surface modification of layered transition-metal oxide cathodes,” *Mater. Today*, vol. 46, pp. 155–182, Jun. 2021, doi: 10.1016/j.mattod.2020.12.017.
 - [5] J. Yuan *et al.*, “Membranes in non-aqueous redox flow battery: A review,” *J. Power Sources*, vol. 500, p. 229983, Jul. 2021, doi: 10.1016/j.jpowsour.2021.229983.
 - [6] “Thermo Scientific Forma Environmental Chamber Model 3911, 311.5 L, Stainless Steel - Incubators, Environmental Chambers.” <https://www.fishersci.com/shop/products/forma-environmental-chamber-model-3911-311-5-l-stainless-steel/13987065> (accessed Apr. 05, 2022).
 - [7] M. M. Flores-Leonar *et al.*, “Materials Acceleration Platforms: On the way to autonomous experimentation,” *Curr. Opin. Green Sustain. Chem.*, vol. 25, p. 100370, Oct. 2020, doi: 10.1016/j.cogsc.2020.100370.
 - [8] E. Stach *et al.*, “Autonomous experimentation systems for materials development: A community perspective,” *Matter*, vol. 4, no. 9, Art. no. 9, Sep. 2021.
 - [9] J. Yano *et al.*, “The case for data science in experimental chemistry: examples and recommendations,” *Nat. Rev. Chem.*, pp. 1–14, Apr. 2022, doi: 10.1038/s41570-022-00382-w.
 - [10] P. Goel *et al.*, “Perovskite materials as superior and powerful platforms for energy conversion and storage applications,” *Nano Energy*, vol. 80, p. 105552, Feb. 2021, doi: 10.1016/j.nanoen.2020.105552.
 - [11] H. Kim, J. S. Han, J. Choi, S. Y. Kim, and H. W. Jang, “Halide Perovskites for Applications beyond Photovoltaics,” *Small Methods*, vol. 2, no. 3, p. 1700310, 2018, doi: 10.1002/smtd.201700310.
 - [12] S. Mazumdar, Y. Zhao, and X. Zhang, “Stability of Perovskite Solar Cells: Degradation Mechanisms and Remedies,” *Front. Electron.*, vol. 2, 2021, Accessed: Jul. 30, 2022. [Online]. Available: <https://www.frontiersin.org/articles/10.3389/felec.2021.712785>
 - [13] A. Urbina, “The balance between efficiency, stability and environmental impacts in perovskite solar cells: a review,” *J. Phys. Energy*, vol. 2, no. 2, p. 022001, Apr. 2020, doi: 10.1088/2515-7655/ab5eee.
 - [14] T. J. Jacobsson *et al.*, “An open-access database and analysis tool for perovskite solar cells based on the FAIR data principles,” *Nat. Energy*, vol. 7, no. 1, Art. no. 1, Jan. 2022, doi: 10.1038/s41560-021-00941-3.
 - [15] M. V. Khenkin *et al.*, “Consensus statement for stability assessment and reporting for perovskite photovoltaics based on ISOS procedures,” *Nat. Energy*, vol. 5, no. 1, Art. no. 1, Jan. 2020, doi: 10.1038/s41560-019-0529-5.
 - [16] W. Fu *et al.*, “Stability of perovskite materials and devices,” *Mater. Today*, Jul. 2022, doi: 10.1016/j.mattod.2022.06.020.
 - [17] C. C. Boyd, R. Cheacharoen, T. Leijtens, and M. D. McGehee, “Understanding Degradation Mechanisms and Improving Stability of Perovskite Photovoltaics,” *Chem. Rev.*, vol. 119, no. 5, pp. 3418–3451, Mar. 2019, doi: 10.1021/acs.chemrev.8b00336.
 - [18] R. Azmi *et al.*, “Damp heat-stable perovskite solar cells with tailored-dimensionality 2D/3D heterojunctions,” *Science*, vol. 376, no. 6588, pp. 73–77, Apr. 2022, doi:

- 10.1126/science.abm5784.
- [19] A. H. Slavney, R. W. Smaha, I. C. Smith, A. Jaffe, D. Umeyama, and H. I. Karunadasa, "Chemical Approaches to Addressing the Instability and Toxicity of Lead–Halide Perovskite Absorbers," *Inorg. Chem.*, vol. 56, no. 1, pp. 46–55, Jan. 2017, doi: 10.1021/acs.inorgchem.6b01336.
 - [20] S. Cheng and H. Zhong, "What Happens When Halide Perovskites Meet with Water?," *J. Phys. Chem. Lett.*, vol. 13, no. 10, pp. 2281–2290, Mar. 2022, doi: 10.1021/acs.jpcclett.2c00166.
 - [21] "Opentrons | Open-source Lab Automation, starting at \$5,000." <https://opentrons.com/> (accessed Nov. 30, 2021).
 - [22] D. C. Florian, M. Odziomek, C. L. Ock, H. Chen, and S. A. Guelcher, "Principles of computer-controlled linear motion applied to an open-source affordable liquid handler for automated micropipetting," *Sci. Rep.*, vol. 10, no. 1, p. 13663, Aug. 2020, doi: 10.1038/s41598-020-70465-5.
 - [23] F. Barthels, U. Barthels, M. Schwickert, and T. Schirmeister, "FINDUS: An Open-Source 3D Printable Liquid-Handling Workstation for Laboratory Automation in Life Sciences," *SLAS Technol. Transl. Life Sci. Innov.*, vol. 25, no. 2, pp. 190–199, Apr. 2020, doi: 10.1177/2472630319877374.
 - [24] M. C. Carvalho and R. H. Murray, "Osmar, the open-source microsyringe autosampler," *HardwareX*, vol. 3, pp. 10–38, Apr. 2018, doi: 10.1016/j.ohx.2018.01.001.
 - [25] M. Shahabi, S. Rafiee, S. S. Mohtasebi, and S. Hosseinpour, "Image analysis and green tea color change kinetics during thin-layer drying," *Food Sci. Technol. Int.*, vol. 20, no. 6, pp. 465–476, Sep. 2014, doi: 10.1177/1082013213492524.
 - [26] A. Antonelli *et al.*, "Automated evaluation of food colour by means of multivariate image analysis coupled to a wavelet-based classification algorithm," *Anal. Chim. Acta*, vol. 515, no. 1, pp. 3–13, Jul. 2004, doi: 10.1016/j.aca.2004.01.005.
 - [27] E. M. Gonçalves, J. Pinheiro, M. Abreu, T. R. S. Brandão, and C. L. M. Silva, "Modelling the kinetics of peroxidase inactivation, colour and texture changes of pumpkin (*Cucurbita maxima* L.) during blanching," *J. Food Eng.*, vol. 81, no. 4, pp. 693–701, Aug. 2007, doi: 10.1016/j.jfoodeng.2007.01.011.
 - [28] H. Landolt, "Ueber die Zeitdauer der Reaction zwischen Jodsäure und schwefliger Säure," *Berichte Dtsch. Chem. Ges.*, vol. 19, no. 1, pp. 1317–1365, 1886, doi: 10.1002/cber.188601901293.
 - [29] L. Madriz, F. M. Cabrerizo, and R. Vargas, "Exploring Chemical Kinetics at Home in Times of Pandemic: Following the Bleaching of Food Dye Allura Red Using a Smartphone," *J. Chem. Educ.*, vol. 98, no. 6, pp. 2117–2121, Jun. 2021, doi: 10.1021/acs.jchemed.0c01427.
 - [30] R. W. G. Hunt and M. R. Pointer, *Measuring Colour*. John Wiley & Sons, 2011.
 - [31] G. D. Finlayson, M. Mackiewicz, and A. Hurlbert, "Color Correction Using Root-Polynomial Regression," *IEEE Trans. Image Process.*, vol. 24, no. 5, pp. 1460–1470, May 2015, doi: 10.1109/TIP.2015.2405336.
 - [32] P. Menesatti, C. Angelini, F. Pallottino, F. Antonucci, J. Aguzzi, and C. Costa, "RGB Color Calibration for Quantitative Image Analysis: The '3D Thin-Plate Spline' Warping Approach," *Sensors*, vol. 12, no. 6, Art. no. 6, Jun. 2012, doi: 10.3390/s120607063.
 - [33] M. I. Asghar, K. Miettunen, S. Mastroianni, J. Halme, H. Vahlman, and P. Lund, "In situ

- image processing method to investigate performance and stability of dye solar cells,” *Sol. Energy*, vol. 86, no. 1, pp. 331–338, Jan. 2012, doi: 10.1016/j.solener.2011.10.006.
- [34] R. R. Naik *et al.*, “Discovering equations that govern experimental materials stability under environmental stress using scientific machine learning,” *Npj Comput. Mater.*, vol. 8, no. 1, Art. no. 1, Apr. 2022, doi: 10.1038/s41524-022-00751-5.
- [35] D. Wu and D.-W. Sun, “Colour measurements by computer vision for food quality control – A review,” *Trends Food Sci. Technol.*, vol. 29, no. 1, pp. 5–20, Jan. 2013, doi: 10.1016/j.tifs.2012.08.004.
- [36] S. G. Hashmi *et al.*, “Long term stability of air processed inkjet infiltrated carbon-based printed perovskite solar cells under intense ultra-violet light soaking,” *J. Mater. Chem. A*, vol. 5, no. 10, pp. 4797–4802, 2017, doi: 10.1039/C6TA10605F.
- [37] “Growth and characterization of a PbI₂ single crystal used for gamma ray detectors - Zhu - 2007 - Crystal Research and Technology - Wiley Online Library.” <https://onlinelibrary.wiley.com/doi/10.1002/crat.200610847> (accessed Apr. 04, 2022).
- [38] M. K. A. Mohammed, A. Al-Mousoi, M. Mehde, and A. Al-Gebori, “Engineered electronic properties of the spin-coated MAPI for hole-transport-free perovskite solar cell (HT-free PSC): Spinning time and PSC performance relationship,” *Chem. Phys. Lett.*, vol. 754, p. 137718, Jun. 2020, doi: 10.1016/j.cplett.2020.137718.
- [39] S. Sun *et al.*, “A data fusion approach to optimize compositional stability of halide perovskites,” *Matter*, vol. 4, no. 4, pp. 1305–1322, Apr. 2021, doi: 10.1016/j.matt.2021.01.008.
- [40] Z. Kolláth, A. Cool, A. Jechow, K. Kolláth, D. Száz, and K. P. Tong, “Introducing the dark sky unit for multi-spectral measurement of the night sky quality with commercial digital cameras,” *J. Quant. Spectrosc. Radiat. Transf.*, vol. 253, p. 107162, Sep. 2020, doi: 10.1016/j.jqsrt.2020.107162.
- [41] “Camera Basics.” https://www.thorlabs.com/newgrouppage9.cfm?objectgroup_id=8962 (accessed Jul. 30, 2022).
- [42] R. J. Sutton *et al.*, “Cubic or Orthorhombic? Revealing the Crystal Structure of Metastable Black-Phase CsPbI₃ by Theory and Experiment,” *ACS Energy Lett.*, vol. 3, no. 8, pp. 1787–1794, Aug. 2018, doi: 10.1021/acsenerylett.8b00672.
- [43] N. Rolston *et al.*, “Rapid Open-Air Fabrication of Perovskite Solar Modules,” *Joule*, vol. 4, no. 12, pp. 2675–2692, Dec. 2020, doi: 10.1016/j.joule.2020.11.001.
- [44] S. Oberloier and J. M. Pearce, “General Design Procedure for Free and Open-Source Hardware for Scientific Equipment,” *Designs*, vol. 2, no. 1, Art. no. 1, Mar. 2018, doi: 10.3390/designs2010002.
- [45] T. Baden, A. M. Chagas, G. Gage, T. Marzullo, L. L. Prieto-Godino, and T. Euler, “Open Labware: 3-D Printing Your Own Lab Equipment,” *PLoS Biol.*, vol. 13, no. 3, p. e1002086, Mar. 2015, doi: 10.1371/journal.pbio.1002086.
- [46] “Stack Overflow - Where Developers Learn, Share, & Build Careers,” *Stack Overflow*. <https://stackoverflow.com/> (accessed Apr. 15, 2022).
- [47] Thingiverse.com, “Thingiverse - Digital Designs for Physical Objects.” <https://www.thingiverse.com/> (accessed Apr. 15, 2022).
- [48] “GrabCAD Makes Additive Manufacturing at Scale Possible.” <https://grabcad.com/> (accessed Apr. 15, 2022).

- [49] J. M. Pearce, "Economic savings for scientific free and open source technology: A review," *HardwareX*, vol. 8, p. e00139, Oct. 2020, doi: 10.1016/j.ohx.2020.e00139.
- [50] "Build software better, together," *GitHub*. <https://github.com> (accessed Apr. 15, 2022).
- [51] "Adafruit Industries, Unique & fun DIY electronics and kits." https://www.adafruit.com/?gclid=Cj0KCQjwr-SSBhC9ARIsANhzu15FYJS0vuUwgW6SCktyHpUVZCvQyBDO4HwqEnpSdShIP5UMHNKhOPYaAuq1EALw_wcB (accessed Apr. 15, 2022).
- [52] "SparkFun Electronics." https://www.sparkfun.com/?gclid=Cj0KCQjwr-SSBhC9ARIsANhzu16y1q_VGacLrdL3DJH6vk5USCryZC46oXuq_FhgPYaDQoM8wYeQj9EaArSIEALw_wcB (accessed Apr. 15, 2022).
- [53] D. B. Straus, S. Guo, A. M. Abeykoon, and R. J. Cava, "Understanding the Instability of the Halide Perovskite CsPbI₃ through Temperature-Dependent Structural Analysis," *Adv. Mater.*, vol. 32, no. 32, p. 2001069, 2020, doi: 10.1002/adma.202001069.
- [54] O. J. Weber *et al.*, "Phase Behavior and Polymorphism of Formamidinium Lead Iodide," *Chem. Mater.*, vol. 30, no. 11, pp. 3768–3778, Jun. 2018, doi: 10.1021/acs.chemmater.8b00862.
- [55] D. Müllner, "Modern hierarchical, agglomerative clustering algorithms." arXiv, Sep. 12, 2011. doi: 10.48550/arXiv.1109.2378.
- [56] Z. Li *et al.*, "Robot-Accelerated Perovskite Investigation and Discovery," *Chem. Mater.*, vol. 32, no. 13, pp. 5650–5663, Jul. 2020, doi: 10.1021/acs.chemmater.0c01153.
- [57] J. Xie *et al.*, "Study on the correlations between the structure and photoelectric properties of CH₃NH₃PbI₃ perovskite light-harvesting material," *J. Power Sources*, vol. 285, pp. 349–353, Jul. 2015, doi: 10.1016/j.jpowsour.2015.03.114.