

Using Microprobe-Capture In-Emitter Elution to Directly Couple Label-Free Optical Sensing  
Technology with Mass Spectrometry for Top-Down Protein Analysis

Ruben Yiqi Luo<sup>1,2</sup>, Samuel Yang<sup>1</sup>

<sup>1</sup>Department of Pathology, School of Medicine, Stanford University, Stanford, CA, USA

<sup>2</sup>Clinical Laboratories, Stanford Health Care, Palo Alto, CA, USA

Corresponding Author: Ruben Yiqi Luo

Address: 3375 Hillview Ave, Palo Alto, CA 94304

Tel: 650-724-1318

Email: [rubenluo@stanford.edu](mailto:rubenluo@stanford.edu)

Key Words: MPIE, Label-Free Optical Sensing Technology, next-generation BLI, Mass  
Spectrometry, Top-Down Protein Analysis

## **Abstract**

Affinity capture of an analyte by a capture agent is one of the most effective sample preparation approaches for protein analytes. We describe a new affinity capture technique for top-down protein analysis, microprobe-capture in-emitter elution (MPIE), which can directly couple a label-free optical sensing technology (next-generation biolayer interferometry, BLI) with MS. In MPIE, an analyte is first captured on the surface of a microprobe while the capture process was monitored in real-time by BLI, and then eluted from the microprobe inside an electrospray emitter. When electrospray is established from the emitter to a mass spectrometer, the analyte is immediately ionized through electrospray ionization (ESI) for MS analysis. By this means, next-generation BLI and MS are directly coupled in the form of MPIE-ESI-MS. The performance of MPIE-ESI-MS was demonstrated by the analysis of A $\beta$  1-40 and Tf using both standard samples and human specimens. In comparison to the conventional affinity capture techniques such as bead-based immunoprecipitation, MPIE innovated the affinity capture methodology by introducing real-time process monitoring and providing binding characteristics of analytes, providing more information-rich experimental results. Thus, MPIE is a valuable addition to the TD-MS sample preparation toolbox, and more applications of MPIE-ESI-MS in top-down protein analysis can be expected.

## **Introduction**

Top-down mass spectrometry (TD-MS), as a mass spectrometry (MS) methodology to analyze a protein in its intact state without prior enzymatic digestion, can be used to elucidate post-

translational modifications and amino acid variations in proteoforms. It has been widely employed in biological research and started being accepted in clinical diagnostics.<sup>1-3</sup> [Hb paper] While it is an ideal tool to analyze intact protein targets, sample preparation, i.e., the procedure to purify analytes and remove interferents from sample matrices, plays an essential role in determining the data quality of TD-MS analysis.<sup>4,5</sup> Among the sample preparation approaches for protein analytes, affinity capture of an analyte by a capture agent is one of the most effective options (also named immunoaffinity capture if the capture agent is an antibody). A well-known example is mass spectrometric immunoassay (MSIA) which uses an antibody immobilized on porous materials as the capture agent.<sup>6</sup> The challenges to the conventional affinity capture techniques lie in the lack of process monitoring. As no signal is generated during the affinity capture process, it may cost significant time and efforts to optimize the experiment conditions, check the affinity capture performance, and troubleshoot when MS responses are weak or absent.

On the other hand, in the research field of biomolecular interactions, label-free optical sensing technologies have been employed as mainstream platforms to identify interacting partners and characterize biologics.<sup>7</sup> A label-free optical sensing technology senses the refractive index change or optical thickness change on a sensing surface caused by biomolecular interactions, achieving real-time measurement without employing a reporter molecule (enzyme, fluorophore, etc.). The real-time monitoring of biomolecular complex formation can provide interaction characteristics such as kinetic and affinity constants. Incorporating a label-free optical sensing technology with MS can be an ideal solution to overcome the challenges to the conventional affinity capture techniques.

In the past decade the label-free optical sensing technologies have advanced from complex fluidics-based platforms to simple dip-and-read sensing microprobes. A novel technology of this kind is called thin-film interferometry (TFI) or next-generation bilayer interferometry (BLI), which utilizes quartz-glass BLI microprobes to measure biomolecular interactions taking place on the microprobe tips. The dip-and-read feature brings flexibility into experiment design: the microprobes loaded with biomolecules can be applied to various sample types for biomolecular interaction measurement and/or affinity capture.<sup>8,9</sup> Thus, next-generation BLI can be a candidate technology to be incorporated with MS. Efforts were made previously to connect traditional BLI (using optical fiber BLI microprobes instead of quartz-glass ones) with MS, however the two technologies were not directly coupled and the analytes must be eluted before MS analysis.<sup>10-12</sup> Because only a tiny amount of analyte (one layer of molecules) could be captured on the surface of a microprobe, the “indirect coupling” required either multiple affinity capture-elution cycles or an additional step of concentration to make up the analyte dilution in elution liquid, resulting in extended experimental procedures.

In this article, we describe a new affinity capture technique for top-down protein analysis, microprobe-capture in-emitter elution (MPIE), which can directly couple next-generation BLI with MS. In MPIE, an analyte is first captured on the surface of a microprobe while the capture process was monitored in real-time by BLI, and then eluted from the microprobe inside an electrospray emitter. When electrospray is established from the emitter to a mass spectrometer, the analyte is immediately ionized through electrospray ionization (ESI) for MS analysis. By this means, next-generation BLI and MS are directly coupled in the form of MPIE-ESI-MS. The

MPIE-ESI-MS can add significant value to regular MS, or more specifically, TD-MS since affinity capture is typically applied to protein analytes and enzymatic digestion is not included.

## **Materials and Methods**

### Materials and Samples

LC-MS grade water, acetonitrile, and formic acid were purchased from Thermo Fisher Scientific (Waltham, MA).  $\beta$ -Amyloid ( $A\beta$ ) 1-40 standard was purchased from Abcam (Cambridge, UK), and a biotinylated mouse monoclonal anti- $A\beta$  IgG antibody (anti- $A\beta$  Ab) from Biolegend (San Diego, CA). Human transferrin (Tf) standard (Tf purified from human serum) was purchased from Sigma-Aldrich (St. Louis, MI), and a mouse monoclonal anti-transferrin IgG antibody (anti-Tf Ab) from Sinobiological (Wayne, PA), and biotinylated using an EZ-Link HPDP-Biotin reagent kit (Waltham, MA). Remnant cerebrospinal fluid (CSF) and serum samples from general patients were obtained from Stanford Health Care, following approved IRB protocols for the use of remnant patient specimens.

### Sample Preparation

$A\beta$  1-40 and Tf were used as model protein targets to study the performance of MPIE-ESI-MS. The  $A\beta$  1-40 standard was first dissolved in DMSO and then diluted in phosphate-buffered saline at pH 7.4 with 0.02% Tween 20 and 0.2% BSA (PBST-B) to make a concentration series of  $A\beta$  1-40 standard samples. The Tf standard was first dissolved in phosphate-buffered saline at pH

7.4 with 0.02% Tween 20 (PBST) and then diluted in PBST to make a concentration series of Tf standard samples. The capture agents anti-A $\beta$  Ab and anti-Tf Ab were diluted in PBST-B to 10  $\mu$ g/ml for use. The A $\beta$  1-40 standard samples were prepared right before use. For A $\beta$  analysis, CSF samples were 1:1 diluted in PBST-B. For Tf analysis, CSF samples were 1:1 diluted in PBST and serum samples were 1:19 diluted in PBST.

### MPIE-ESI-MS Instrumentation

A Gator Plus analyzer (Gator Bio, Palo Alto, CA) was employed to carry out the BLI-based affinity capture in MPIE-ESI-MS experiments. Cylindrical quartz-glass BLI microprobes with 1 mm diameter were used. An ECE-001 capillary electrophoresis (CE) instrument and an EMASS-II ESI ion source (CMP Scientific, Brooklyn, NY) were employed to carry out MPIE and combine it with MS. A glass electrospray emitter with 1.5 mm O.D. and 1.17 mm I.D. (CMP Scientific, Brooklyn, NY) was used for MPIE. It has a regular open end and a tapered open end with a tip orifice that has a diameter of 20-30  $\mu$ m. A fused-silica capillary (360  $\mu$ m O.D., 50  $\mu$ m I.D., 100 cm) was used to deliver an elution liquid (80% acetonitrile and 2% formic acid in water) into the emitter. An Orbitrap Q-Exactive Plus mass spectrometer (Thermo Fisher Scientific, San Jose, CA) was employed to carry out MS analysis.

### MPIE-ESI-MS Experiment

An MPIE-ESI-MS experiment consists of two components: BLI-based affinity capture and in-emitter elution ESI-MS. The BLI-based affinity capture was implemented in 3 steps: (1) a BLI

microprobe pre-coated with streptavidin was dipped into a capture agent (anti-A $\beta$  Ab or anti-Tf Ab) solution for 10 min to load the capture agent; (2) the microprobe was dipped into a sample for 10 min to capture the corresponding analyte (A $\beta$  or Tf) and then rinsed in the running buffer (PBST-B for A $\beta$  analysis or PBST for Tf analysis) for 1 min to remove non-specifically bound molecules. The in-emitter elution ESI-MS was implemented in 6 steps: (1) an electrospray emitter was filled with a sheath liquid (10 mM ammonium formate in water); (2) a microprobe after affinity capture was rinsed in the sheath liquid for 10 s, inserted into the emitter through the regular open end, and settled towards the tapered end by gravity; (3) the emitter was mounted to the ESI ion source; (4) the elution liquid-delivering capillary was inserted into the emitter through the regular open end and positioned right behind the microprobe; (5) a positive voltage was applied to the sheath liquid in the emitter to establish electrospray; (6) MS data acquisition was initiated, and injection of the elution liquid was started subsequently. The emitter was placed ~2 mm away from the mass spectrometer inlet, and the electrospray voltage was set at 2.2 kV. The injection of the elution liquid was driven by 5 psi pneumatic pressure. The parts described above are shown in Figure 1A. The procedures of running BLI-based affinity capture and setting up the in-emitter elution ESI-MS are illustrated in Figure 1B and Figure 1C, respectively.

The MS parameters for A $\beta$  analysis were ion-transfer capillary temperature 320°C, S-lens RF level 50, and number of microscans 5. Full MS dd-MS<sup>2</sup> mode was applied: primary mass spectra acquired in positive polarity at resolution 140K; stepped normalized collision energy 20, 30, and 40 for fragmentation; secondary mass spectra acquired for the top 5 abundant precursor ions at resolution 70K. When analyzing CSF samples, targeted-SIM dd-MS<sup>2</sup> mode was used to increase the analytical sensitivity. The isolation window was set at m/z 4.0 and the number of microscans

was increased to 10. The MS parameters for Tf analysis were ion-transfer capillary temperature 350°C, S-lens RF level 50, and number of microscans 10. Primary mass spectra were acquired in positive polarity at resolution 17.5K.

### Data Analysis

The acquired data in each MPIE-ESI-MS experiment was viewed as a time trace of MS responses, and the elution time window of an analyte was identified by checking the molecular ions of the analyte at each time point. The data in the elution time window were selected for deconvolution using Biopharma Finder 4.1 (Thermo Fisher Scientific, San Jose, CA) with the Xtract algorithm for A $\beta$  analysis and the ReSpect algorithm for Tf analysis. MS peaks of analytes were displayed in deconvoluted spectra at uncharged state showing monoisotopic molecular masses with the Xtract algorithm and average molecular masses with the ReSpect algorithm.

### **Results and Discussion**

The performance of MPIE-ESI-MS was demonstrated by the analysis of A $\beta$  1-40 and Tf, which are typical human proteins and used as clinical diagnostic markers. A $\beta$  1-40 is a 40-amino acid small protein (or peptide) closely related to Alzheimer's disease.<sup>13</sup> Tf is a 679-amino acid glycosylated large protein playing an essential role in iron metabolism, and its proteoforms are used to diagnose CSF leak.<sup>14</sup> A concentration series of A $\beta$  1-40 standard samples at 3.3, 1.1, 0.37, and 0.12  $\mu\text{g/ml}$  were analyzed by MPIE-ESI-MS, as shown in Figure 2A. Similarly, a



concentration series of Tf standard samples at 1.0, 0.50, 0.25, 0.13  $\mu\text{g/ml}$ , and 0.063  $\mu\text{g/ml}$  were analyzed by MPIE-ESI-MS, as shown in Figure 3A. In both cases a blank sample (running buffer) was employed as the reference for the label-free optical sensing measurement and the negative control for the MS analysis. Real-time monitoring of affinity capture process was implemented in the next-generation BLI analyzer, and the reference-subtracted time traces of label-free optical sensing responses (sensorgrams) were obtained. The sensorgrams showed the association phase (analyte-capturing phase) and dissociation phase (sensing surface rinsed in the running buffer). The intact-protein MS analysis of A $\beta$  1-40 standard samples showed a dominant MS peak at 4327.1 Da and that of Tf standard samples showed a dominant MS peak at 79554 Da in deconvoluted mass spectra. The blank samples showed only noises in the raw mass spectra and no MS peak after deconvolution. In the A $\beta$  1-40 analysis, the dominant analyte should be A $\beta$  1-40 as the measured molecular mass (monoisotopic mass) matched the theoretical molecular mass 4327.148 Da calculated from its primary structure. The assignment could be confirmed by MS<sup>2</sup> fragmentation: the MS<sup>2</sup> analysis of the +4 precursor ion of A $\beta$  1-40 ( $m/z$  1083.3) in a A $\beta$  1-40 standard sample is shown in Figure 2B. In the deconvoluted MS<sup>2</sup> mass spectrum, 37 b-fragments and 9 y-fragments were identified by matching their masses to the predicted fragments derived from the amino acid sequence of A $\beta$  1-40, resulting in a sequence coverage of 95%. Moreover, a minor MS peak at 4349.1 Da was observed in some deconvoluted mass spectra, which was probably the sodium adduct of A $\beta$  1-40. In the Tf analysis, since it is known that a tetrasialo-Tf proteoform predominates in normal human serum and the Tf standard was purified from human serum, the dominant analyte was likely the major serum Tf proteoform as the measured molecular mass (average mass) matched the theoretical mass 79554.71 Da calculated from its primary structure with the reported N-glycans of the tetrasialo-Tf.<sup>15,16</sup> Note that the

eluted Tf molecules were denatured and iron-free since a protein-denaturing elution liquid was used.

A sensorgram not only indicates the amount of the analyte captured on a microprobe, but it can also be fitted to the Langmuir molecular interaction model to obtain the kinetic and affinity constants between the two binding partners (Langmuir model explained in supporting information).<sup>17</sup> Using the sensorgrams in Figure 2A and Figure 3A, the association kinetic constants ( $k_a$ ) and dissociation kinetic constants ( $k_d$ ) could be measured, and the affinity constant (dissociation equilibrium constant  $K_D$ ) could be calculated using the kinetic constants. Regarding the binding pair of anti-A $\beta$  Ab and A $\beta$  1-40,  $k_a$  was  $7.4 \times 10^5 \text{ M}^{-1}\text{s}^{-1}$ ,  $k_d$  was  $4.9 \times 10^{-3} \text{ s}^{-1}$ , and  $K_D$  was  $6.6 \times 10^{-8} \text{ M}$ . Regarding the binding pair of anti-Tf Ab and Tf,  $k_a$  was  $2.8 \times 10^5 \text{ M}^{-1}\text{s}^{-1}$ ,  $k_d$  was  $1.1 \times 10^{-3} \text{ s}^{-1}$ , and  $K_D$  was  $3.9 \times 10^{-9} \text{ M}$ . The affinity constants were in the regular range of mouse monoclonal antibodies, and consistent with the knowledge that antibodies bind more strongly to larger-sized antigens.

The analysis of the Tf standard samples also demonstrated the analytical sensitivity of MPIE-ESI-MS. Because only a tiny amount of analyte (one layer of molecules) could be captured on the surface of a microprobe, the use of the particular electrospray emitter was crucial: the captured analyte on a microprobe was eluted into the tiny space at the tapered end of the electrospray emitter, which was about  $0.8 \mu\text{l}$  calculated from the dimensions; the tiny space enforced restricted dispersion of eluted analyte to enhance the analytical sensitivity of MS analysis. As demonstrated in Figure 3A, the limit of detection for the Tf standard was at least  $0.063 \mu\text{g/ml}$ , which corresponded to a saturation rate of anti-Tf Ab at 17% (calculation in

supporting information). Provided that there was one layer of anti-Tf Ab molecules on the surface of a microprobe to capture Tf molecules and the maximum density for a typical protein on a label-free optical sensing surface is 1-2 ng/mm<sup>2</sup>,<sup>18</sup> the amount of anti-Tf Ab on a microprobe (tip area 3 mm<sup>2</sup>) should be within 40 fmol and the captured Tf molecules should be no more than 7 fmol, which was an very low quantity. In fact, limited capture capacity of label-free optical sensing devices was a major barrier that hindered the combination of label-free optical sensing technologies and MS in the past. The feature of restricted dispersion of eluted analyte in MPIE-ESI-MS facilitated exceedingly good analytical sensitivity to successfully couple a label-free optical sensing technology with MS.

MPIE-ESI-MS was applied to human specimens to evaluate its applicability to clinical diagnostics. For A $\beta$  1-40 analysis, two normal CSF samples drawn from individuals without Alzheimer's disease were tested. Given the normal A $\beta$  1-40 concentration in CSF at the level of 10 ng/ml and the affinity constant ( $K_D$ ) of the binding pair at  $6.6 \times 10^{-8}$  M,<sup>19</sup> the saturation of anti-A $\beta$  Ab was around 3.4% (calculation in supporting information). As the low saturation rate of capture agent limited the amount of A $\beta$  1-40 captured on the microprobes, targeted-SIM dd-MS<sup>2</sup> mode was used to increase the analytical sensitivity of the MS analysis. A $\beta$  1-40 was successfully detected in the two normal CSF samples, as shown in Figure 2C. For Tf analysis, a serum sample and a CSF sample drawn from the same individual were tested. In Figure 3B, the deconvoluted mass spectrum of the serum sample showed a dominant MS peak at 79554 Da and smaller MS peaks around it. The MS peaks should be mainly serum Tf proteoforms and the dominant MS peak at 79554 Da was the major serum Tf proteoform, consistent with that measured from the Tf standard samples. In Figure 3C, the deconvoluted mass spectrum of the

CSF sample showed a significant MS peak at 78008 Da and smaller MS peaks around it, in addition to the serum Tf proteoforms. The MS peaks around 78008 Da should be mainly brain Tf proteoforms, consistent with the reports that two types of Tf proteoforms (serum and brain) are present in CSF.<sup>20,21</sup> The test results of the human specimens demonstrated that MPIE-ESI-MS has the potential to be used as a clinical diagnostic tool.

It should be noted that the capture agents in MPIE are not limited to antibodies. Other biologics that bind to a specific target with sufficient affinity can be used, such as lectins or enzymes. It was demonstrated in the analysis of A $\beta$  1-40 and Tf that binding characteristics of the binding pair (capture agent and analyte) could be obtained together with the MS analysis of the analyte in a single MPIE-ESI-MS experiment. Combining the binding characteristics with the structural information obtained from MS analysis can add significant value to the study of unknown targets. In addition, as label-free optical sensing devices are equipped with optimal surface chemistry to mitigate non-specific binding of interferents,<sup>18,22</sup> the performance of affinity capture in MPIE is more advantageous than the conventional affinity capture techniques. Thus, MPIE-ESI-MS can be a useful tool for biological research.

## **Conclusion**

It was demonstrated that the affinity capture technique MPIE has the ability to directly couple a label-free optical sensing technology (next-generation BLI) with MS. The employment of next-generation BLI brings unique advantages to top-down protein analysis: (1) BLI allows for effective step-by-step optimization of affinity capture conditions, while MS analysis is not

required; (2) real-time monitoring of affinity capture process provides estimated amount of captured analyte for every sample, serving as a means of quality control; (3) captured analyte is eluted into a tiny space at the tapered end of the electrospray emitter to enhance the analytical sensitivity of MS analysis. In comparison to the conventional affinity capture techniques such as bead-based immunoprecipitation, MPIE innovates the affinity capture methodology by introducing real-time process monitoring and providing binding characteristics of analytes, offering more information-rich experimental results. Thus, MPIE is a valuable addition to the TD-MS sample preparation toolbox, and more applications of MPIE-ESI-MS in top-down protein analysis can be expected.

## Acknowledgment

The authors thank Gator Bio (Palo Alto, CA) and CMP Scientific (Brooklyn, NY) for kindly providing equipment and consumables for this research.

## References

- (1) Catherman, A. D.; Skinner, O. S.; Kelleher, N. L. Top Down Proteomics: Facts and Perspectives. *Biochemical and Biophysical Research Communications* **2014**, *445* (4), 683–693. <https://doi.org/10.1016/j.bbrc.2014.02.041>.
- (2) Tiambeng, T. N.; Tucholski, T.; Wu, Z.; Zhu, Y.; Mitchell, S. D.; Roberts, D. S.; Jin, Y.; Ge, Y. Analysis of Cardiac Troponin Proteoforms by Top-down Mass Spectrometry. In *Methods in Enzymology*; Elsevier, 2019; Vol. 626, pp 347–374. <https://doi.org/10.1016/bs.mie.2019.07.029>.
- (3) Ntai, I.; Fornelli, L.; DeHart, C. J.; Hutton, J. E.; Doubleday, P. F.; LeDuc, R. D.; van Nispen, A. J.; Fellers, R. T.; Whiteley, G.; Boja, E. S.; Rodriguez, H.; Kelleher, N. L. Precise Characterization of KRAS4b Proteoforms in Human Colorectal Cells and Tumors Reveals Mutation/Modification Cross-Talk. *Proc. Natl. Acad. Sci. U.S.A.* **2018**, *115* (16), 4140–4145. <https://doi.org/10.1073/pnas.1716122115>.
- (4) Donnelly, D. P.; Rawlins, C. M.; DeHart, C. J.; Fornelli, L.; Schachner, L. F.; Lin, Z.; Lippens, J. L.; Aluri, K. C.; Sarin, R.; Chen, B.; Lantz, C.; Jung, W.; Johnson, K. R.; Koller, A.; Wolff, J. J.; Campuzano, I. D. G.; Auclair, J. R.; Ivanov, A. R.; Whitelegge, J. P.; Paša-Tolić, L.; Chamot-Rooke, J.; Danis, P. O.; Smith, L. M.; Tsybin, Y. O.; Loo, J. A.;

- Ge, Y.; Kelleher, N. L.; Agar, J. N. Best Practices and Benchmarks for Intact Protein Analysis for Top-down Mass Spectrometry. *Nat Methods* **2019**, *16* (7), 587–594. <https://doi.org/10.1038/s41592-019-0457-0>.
- (5) Padula, M.; Berry, I.; O'Rourke, M.; Raymond, B.; Santos, J.; Djordjevic, S. P. A Comprehensive Guide for Performing Sample Preparation and Top-Down Protein Analysis. *Proteomes* **2017**, *5* (4), 11. <https://doi.org/10.3390/proteomes5020011>.
- (6) Trenchevska, O.; Nelson, R.; Nedelkov, D. Mass Spectrometric Immunoassays in Characterization of Clinically Significant Proteoforms. *Proteomes* **2016**, *4* (1), 13. <https://doi.org/10.3390/proteomes4010013>.
- (7) Sun, Y.-S. OPTICAL BIOSENSORS FOR LABEL-FREE DETECTION OF BIOMOLECULAR INTERACTIONS. *Instrumentation Science & Technology* **2014**, *42* (2), 109–127. <https://doi.org/10.1080/10739149.2013.843060>.
- (8) Luo, Y. R.; Chakraborty, I.; Lazar-Molnar, E.; Wu, A. H. B.; Lynch, K. L. Development of Label-Free Immunoassays as Novel Solutions for the Measurement of Monoclonal Antibody Drugs and Antidrug Antibodies. *Clinical Chemistry* **2020**, *66* (10), 1319–1328. <https://doi.org/10.1093/clinchem/hvaa179>.
- (9) Luo, Y. R.; Yun, C.; Chakraborty, I.; Wu, A. H. B.; Lynch, K. L. A SARS-CoV-2 Label-Free Surrogate Virus Neutralization Test and a Longitudinal Study of Antibody Characteristics in COVID-19 Patients. *J Clin Microbiol* **2021**, *59* (7). <https://doi.org/10.1128/JCM.00193-21>.
- (10) Jung, V.; Roger, K.; Chhuon, C.; Pannetier, L.; Lipecka, J.; Gomez, J. S.; Chappert, P.; Charbit, A.; Guerrero, I. C. BLI-MS: Combining Biolayer Interferometry and Mass Spectrometry. *Proteomics* **2022**, 2100031. <https://doi.org/10.1002/pmic.202100031>.
- (11) Machen, A. J.; O'Neil, P. T.; Pentelute, B. L.; Villar, M. T.; Artigues, A.; Fisher, M. T. Analyzing Dynamic Protein Complexes Assembled On and Released From Biolayer Interferometry Biosensor Using Mass Spectrometry and Electron Microscopy. *JoVE* **2018**, No. 138, 57902. <https://doi.org/10.3791/57902>.
- (12) Zhang, G.; Li, C.; Quartararo, A. J.; Loas, A.; Pentelute, B. L. Automated Affinity Selection for Rapid Discovery of Peptide Binders. *Chem. Sci.* **2021**, *12* (32), 10817–10824. <https://doi.org/10.1039/D1SC02587B>.
- (13) Murphy, M. P.; LeVine, H. Alzheimer's Disease and the Amyloid- $\beta$  Peptide. *JAD* **2010**, *19* (1), 311–323. <https://doi.org/10.3233/JAD-2010-1221>.
- (14) Papadea, C.; Schlosser, R. J. Rapid Method for B2-Transferrin in Cerebrospinal Fluid Leakage Using an Automated Immunofixation Electrophoresis System. *Clinical Chemistry* **2005**, *51* (2), 464–470. <https://doi.org/10.1373/clinchem.2004.042697>.
- (15) de Jong, G.; van Eijk, H. G. Microheterogeneity of Human Serum Transferrin: A Biological Phenomenon Studied by Isoelectric Focusing in Immobilized PH Gradients. *Electrophoresis* **1988**, *9* (9), 589–598. <https://doi.org/10.1002/elps.1150090921>.
- (16) de Jong, G.; van Noort, W. L.; van Eijk, H. G. Carbohydrate Analysis of Transferrin Subfractions Isolated by Preparative Isoelectric Focusing in Immobilized PH Gradients. *Electrophoresis* **1992**, *13* (1), 225–228. <https://doi.org/10.1002/elps.1150130146>.
- (17) *Label-Free Biosensors: Techniques and Applications*, 1st ed.; Cooper, M. A., Ed.; Cambridge University Press, 2009. <https://doi.org/10.1017/CBO9780511626531>.
- (18) *Handbook of Surface Plasmon Resonance*; Schasfoort, R. B. M., Tudos, A. J., Eds.; RSC Pub: Cambridge, UK, 2008.

- (19) Lehmann, S.; Dumurgier, J.; Ayrygnac, X.; Marelli, C.; Alcolea, D.; Ormaechea, J. F.; Thouvenot, E.; Delaby, C.; Hirtz, C.; Vialaret, J.; Ginestet, N.; Bouaziz-Amar, E.; Laplanche, J.-L.; Labauge, P.; Paquet, C.; Lleo, A.; Gabelle, A.; for the Alzheimer's Disease Neuroimaging Initiative (ADNI). Cerebrospinal Fluid A Beta 1–40 Peptides Increase in Alzheimer's Disease and Are Highly Correlated with Phospho-Tau in Control Individuals. *Alz. Res Therapy* **2020**, *12* (1), 123. <https://doi.org/10.1186/s13195-020-00696-1>.
- (20) Hoffmann, A.; Nimtz, M.; Getzlaff, R.; Conradt, H. S. 'Brain-Type' *N*-Glycosylation of Asialo-Transferrin from Human Cerebrospinal Fluid. *FEBS Letters* **1995**, *359* (2–3), 164–168. [https://doi.org/10.1016/0014-5793\(95\)00034-7](https://doi.org/10.1016/0014-5793(95)00034-7).
- (21) Hoshi, K.; Matsumoto, Y.; Ito, H.; Saito, K.; Honda, T.; Yamaguchi, Y.; Hashimoto, Y. A Unique Glycan-Isoform of Transferrin in Cerebrospinal Fluid: A Potential Diagnostic Marker for Neurological Diseases. *Biochimica et Biophysica Acta (BBA) - General Subjects* **2017**, *1861* (10), 2473–2478. <https://doi.org/10.1016/j.bbagen.2017.07.005>.
- (22) Homola, J. Surface Plasmon Resonance Sensors for Detection of Chemical and Biological Species. *Chem. Rev.* **2008**, *108* (2), 462–493. <https://doi.org/10.1021/cr068107d>.

### Conflicts of Interest

No conflict for all the authors.

### Figures


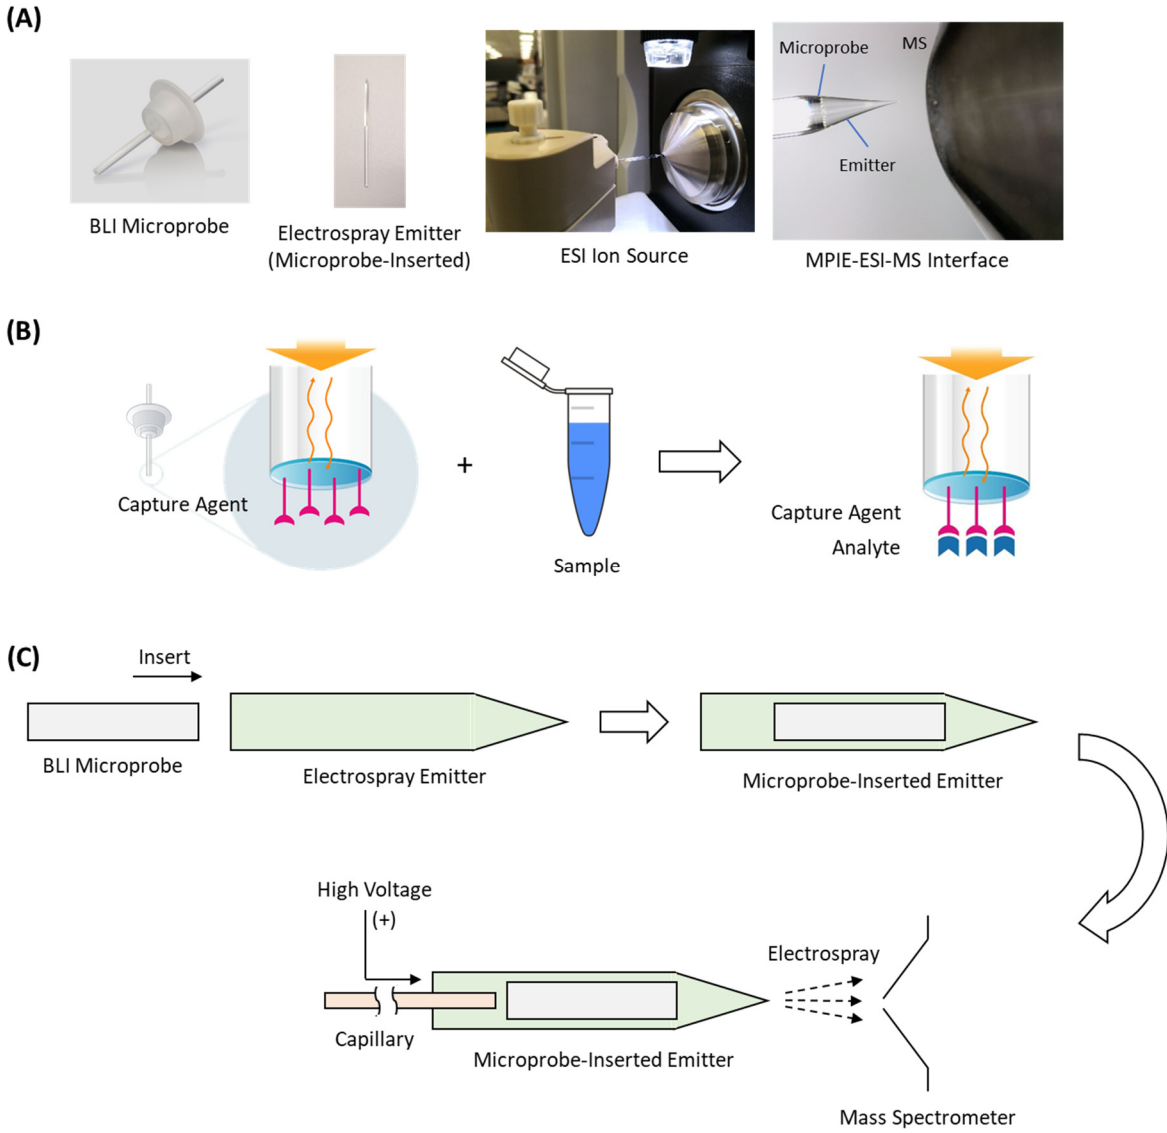



Figure 1. (A) Pictures of BLI microprobe, electro spray emitter, ESI ion source, and MPIE-ESI-MS interface under stereoscope. (B) Illustration of running BLI-based affinity capture. (C) Illustration of setting up the in-emitter elution ESI-MS.



(A)

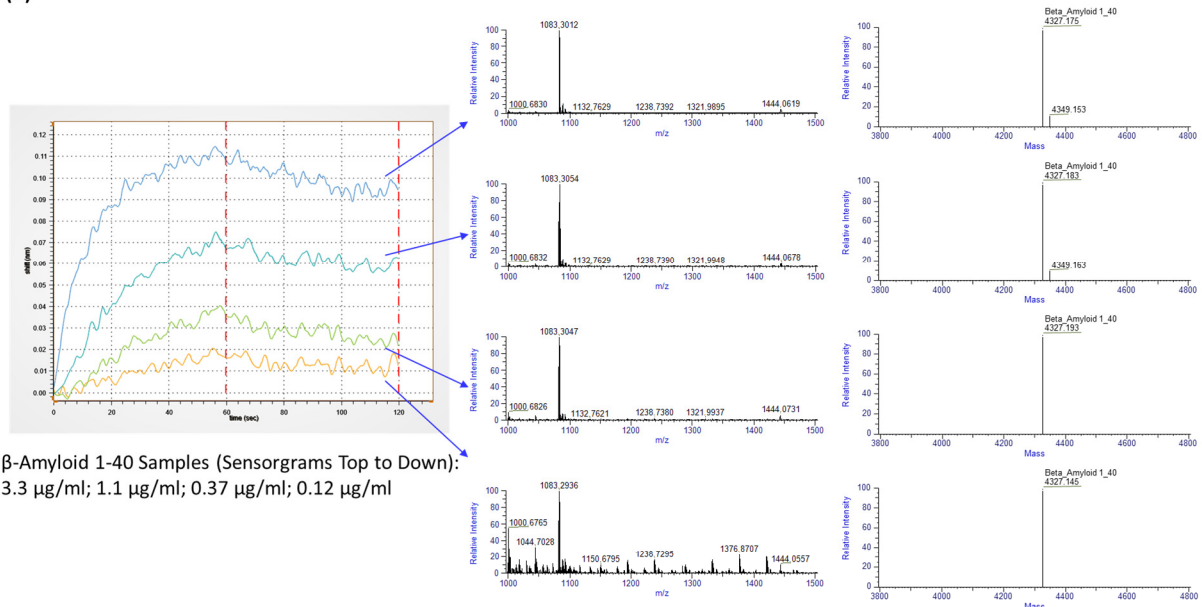

(B)

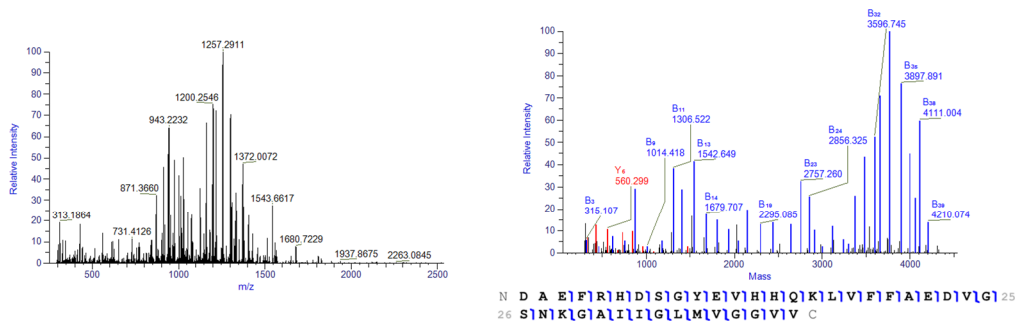

(C)


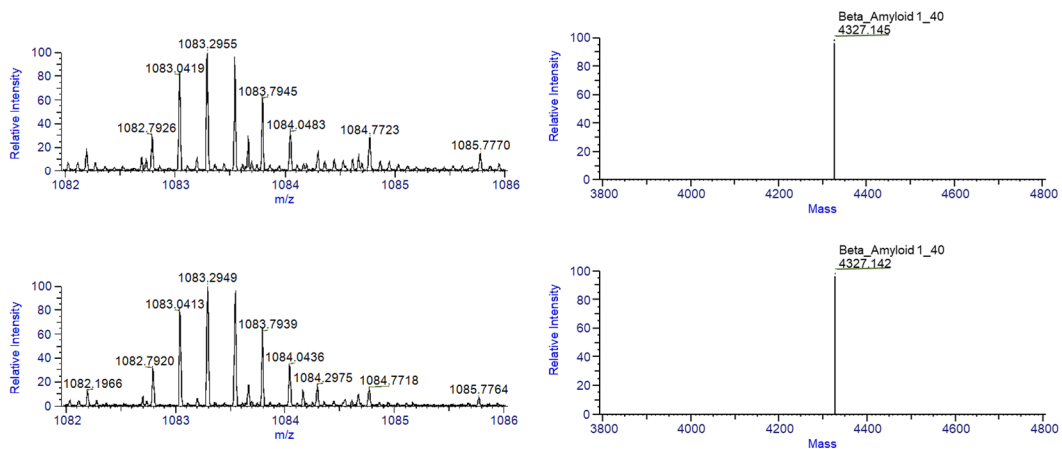



Figure 2. MPE-ESI-MS analysis of A $\beta$  1-40. (A) A concentration series of A $\beta$  1-40 standard samples: sensorgrams obtained from the 4 microprobes measuring 4 samples at different concentrations (left); raw mass spectra and deconvoluted mass spectra of eluted A $\beta$  1-40

molecules from the 4 microprobes (right), showing A $\beta$  1-40 (4327.1 Da) and probably the sodium adduct of A $\beta$  1-40 (4349.1 Da). (B) MS<sup>2</sup> analysis of the +4 precursor ion of A $\beta$  1-40 (m/z 1083.3) in a A $\beta$  1-40 standard sample: raw MS<sup>2</sup> mass spectrum (left) and deconvoluted MS<sup>2</sup> mass spectrum (right) of A $\beta$  1-40 fragments, showing the identified fragments of A $\beta$  1-40. (C) Two normal CSF samples: raw mass spectra (left) and deconvoluted mass spectra (right) of eluted A $\beta$  1-40 molecules, showing that A $\beta$  1-40 in CSF could be captured and analyzed.

(A)

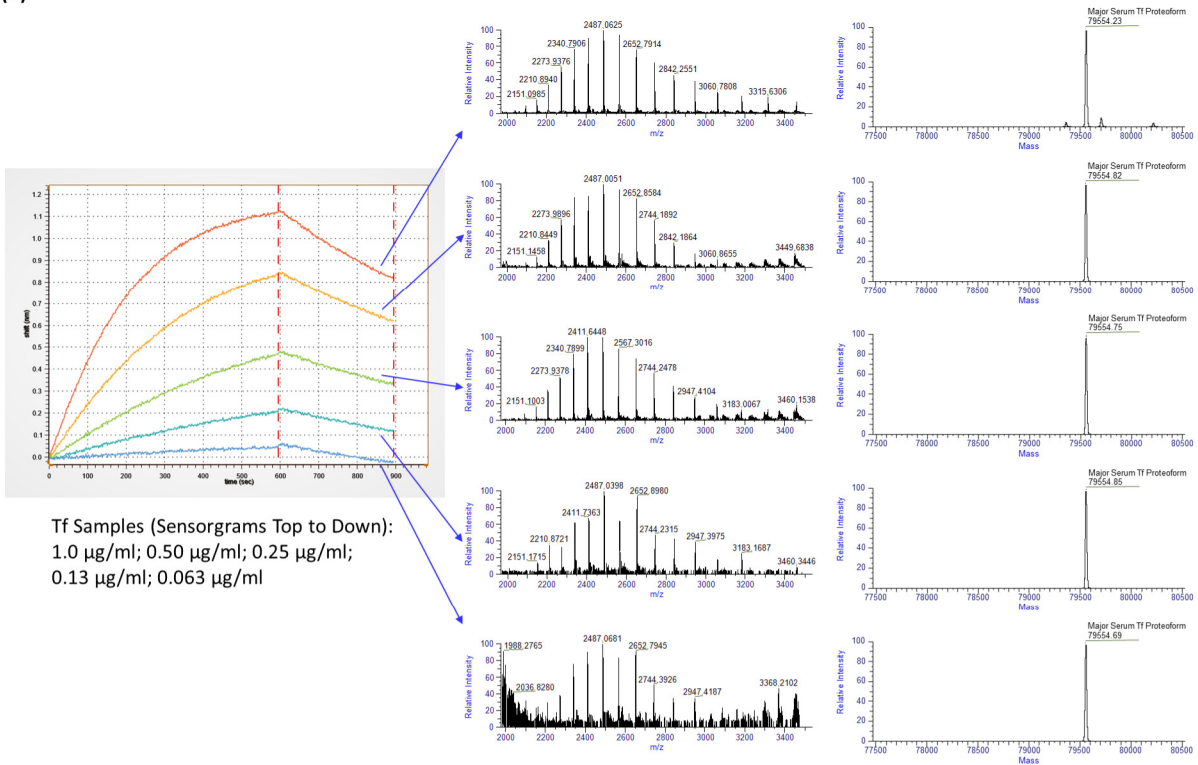

(B)

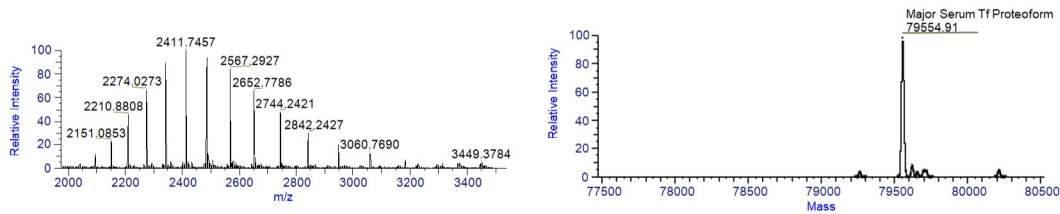

(C)

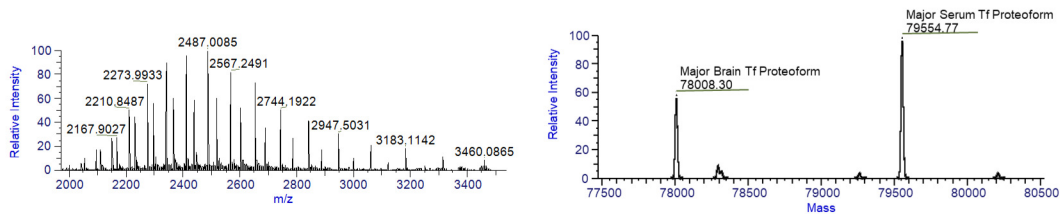


Figure 3. MPIE-ESI-MS analysis of Tf. (A) A concentration series of Tf standard samples: sensorgrams obtained from the 5 microprobes measuring 5 samples at different concentrations (left); MS raw mass spectra and deconvoluted mass spectra of eluted Tf molecules from the 5 microprobes (right), showing the major serum Tf proteoform (79554 Da). (B) A serum sample: raw mass spectrum (left) and deconvoluted mass spectrum (right) of eluted Tf molecules, showing the major (79554 Da) and minor serum Tf proteoforms. (C) A CSF sample: raw mass

spectrum (left) and deconvoluted mass spectrum (right) of eluted Tf molecules, showing the major (79554 Da) and minor serum Tf proteoforms as well as the major (78008 Da) and minor brain Tf proteoforms. The serum and CSF samples were drawn from the same individual.

## Supporting Information

### Langmuir molecular interaction model

In label-free analysis, a sensorgram shows the binding kinetics between two binding partners (analyte and capture agent), including association phase and dissociation phase. The binding kinetics can be described by the Langmuir molecular interaction model and the related equations. The kinetic and affinity constants can be obtained by fitting the sensorgram to the equations.

#### Langmuir Molecular Interaction Model



Association Phase Kinetic Equation:

$$\frac{d[AB]}{dt} = k_1[A][B] - k_2[B]$$

$$K_D = \frac{k_2}{k_1}$$

Association Phase Kinetic Equation:

$$[AB] = \frac{[A][B]_0}{K_D + [A]} [1 - e^{-(k_1[A] + k_2)t}]$$

Dissociation Phase Kinetic Equation:

$$[AB] = [AB]_0 e^{-k_2 t}$$

$k_1$  – association kinetic constant,  $k_2$  – dissociation kinetic constant,  $K_D$  – equilibrium constant,

$[A]$  – concentration of analyte in solution,  $[B]$  – density of unbound capture agent on microprobe

surface,  $[B]_0$  – density of all capture agent on microprobe surface,  $[AB]$  – density of complex on

microprobe surface,  $[AB]_0$  – density of complex on microprobe surface at the starting point of dissociation phase

#### Saturation rate of capture agent on the surface of a microprobe

In label-free analysis, the density of the complex formed by an analyte and a capture agent can be calculated using the Langmuir molecular interaction model. At equilibrium, the density is described by this equation.

$$[AB] = \frac{[A][B]_0}{K_D + [A]}$$

The saturation rate of the capture agent can be calculated by this equation.

$$\frac{[AB]}{[B]_0} = \frac{[A]}{K_D + [A]}$$

In the MPIE-ESI-MS analysis of the 0.063  $\mu\text{g/ml}$  Tf standard sample, given the concentration of analyte (Tf) at the limit of detection 0.063  $\mu\text{g/ml}$  (0.79 nM) and the equilibrium constant  $K_D$  at  $3.9 \times 10^{-9}$  M, the saturation rate was 17%.

In the MPIE-ESI-MS analysis of  $A\beta$  1-40 in normal CSF samples, given the concentration of analyte ( $A\beta$  1-40) at the level of 10 ng/ml (2.3 nM) and the equilibrium constant  $K_D$  at  $6.6 \times 10^{-8}$  M, the saturation rate was 3.4%.