


Digitisation of a Modular Plug and Play 3D Printed Continuous Flow System for Chemical Synthesis

Mireia Benito Montaner, Matthew R. Penny and Stephen T. Hilton

UCL School of Pharmacy, 29-39 Brunswick Square, London WC1N 1AX

Abstract: We describe the development of a digital modular 3D printed continuous flow system to carry out both classical and photochemical synthesis that uses a novel PC based software interface.

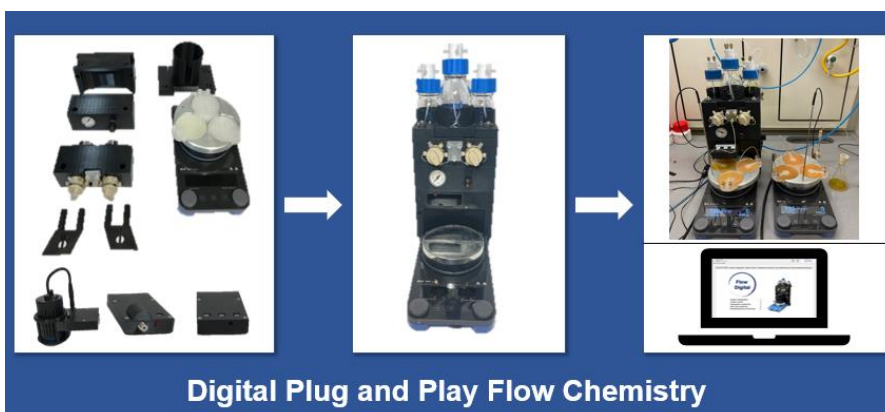

Using this system, we describe how we were able to both control and monitor reaction conditions at the same time. The system integrates in-line sensors via a simple cassette based system that is analogous to a games console enabling hot-swapping of modules by a user. To control the system, an PC-interface platform was created to automate the control of the system functionality, as well as the reporting of sensor parameters. The utility of the system was demonstrated by performing a series of reactions highlighting the importance that precise control of solvent flow rate and accurate reporting of reaction temperatures can have on standardization and reproducibility and that the system can be easily modified to allow for scale-up synthesis.

Despite the clear advantages of continuous flow over batch chemical syntheses, batch processes remain, in general, a standard “go-to” option for new Active Pharmaceutical Ingredients (APIs) syntheses for most chemists. Notwithstanding the advantages of continuous flow, chemists often reach for batch processes due to their prior training and familiarity with the associated set-up and procedures as well as the availability of the requisite equipment needed to carry out a reaction. This problem arises from a deficit of continuous flow experimental training at University level and a lack of continuous flow equipment in most laboratories due to the high costs of the commercial systems.¹ In order to make flow chemistry more accessible and to increase the availability of flow systems, researchers have sought to design and develop 3D printed continuous flow systems as well as alternative low-cost syringe pump continuous flow systems with a number of recent reports in the literature.^{2,3}

Adaptations of existing continuous flow equipment to address these deficits and reduce costs have utilised 3D printed polypropylene (PP) column reactors in the synthesis of bicyclic heterocycles and complex tetracycles,⁴ or the use of stainless-steel flow reactors by Maier as

examples.⁵ Notable efforts in the development of integrated digital continuous flow systems by others have focussed on 3D printed syringe pumps and continuous flow systems as reported by Saggiomo, Cronin and Neumaier amongst others.⁶ Alongside the growing popularity of the maker culture exemplified by 3D printing which has heavily impacted the field of chemistry and has reduced these deficits and improved access to continuous flow equipment, the use of open-source software has also been rapidly incorporated and reported within the scientific community in the development of low-cost instrumentation. Through open-source electronics, such as Arduino and Raspberry Pi microcontrollers, chemistry researchers have become more digitally oriented, resulting in improved reporting and acquisition, as well as automation and remote collection of research data. Furthermore, the use of open-source software combined with 3D printed equipment has allowed scientists to realise the development of low-cost laboratory systems tailored to meet researcher's needs, thus circumventing the limitations of commercial laboratory equipment, whose functionalities and properties cannot normally be modified. A recent overview of the various types of microcontrollers used in the scientific field has been described by Prabhu and Urban and there have been a number of recent articles demonstrating how low-cost electronics can be integrated with chemical synthesis and continuous flow synthesis for substance detection.⁷⁻²⁰

System Design

As a result of experiencing the high costs of continuous flow systems along with prior 3D printing research, in 2019, the Hilton group designed and introduced a low-cost 3D-printed modular pressure driven continuous flow system that chemists could use and integrate with existing laboratory equipment (Figure 1A).^{21,22} Whilst the system was designed to meet the entry needs of a continuous flow system similar to commercially available congeners, it lacked the ability to monitor reaction parameters in real time, which is essential if chemists are to enhance reproducibility and standardisation of reaction conditions in the literature. In order to address these deficits and to provide a standardised system for reporting continuous flow data, we now wish to describe our research into a modular digitized version of our previous 3D printed system that now incorporates Arduino open-source electronics and a simple-to-use PC linked software interface to accurately monitor the temperature and flow rate throughout a reaction and that allows for facile variable scalable syntheses (Figure 1B, C).

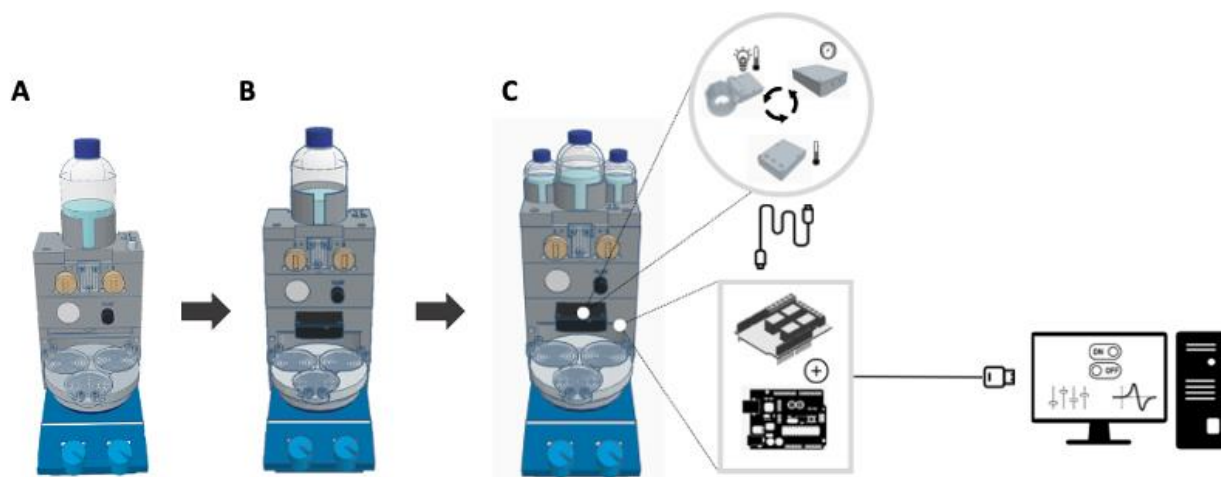


Figure 1: Tinkercad representative design of the proposed modular continuous flow chemistry system. A) Analog system. B) Digital system. C) Scale-up version of the digital system.

The analogue system previously reported by the group was designed to be modular in nature so that it could be easily assembled and disassembled for use with any stirrer hotplate in the laboratory and upgraded by users as desired. Amongst the modules of this system are a solvent block that fits a 500 mL Duran pressure bottle, an injection block containing two 2 mL loop injection valves and a 3D printed mixing chip, which then connects to the 3D printed reactors, a flow unit to regulate the pressure applied, and a base block that provides compressed air to power and run the whole system.²¹ In order to digitise the flow system and monitor the reaction's temperature or flow rate, we envisaged that a range of in-line sensors could be added in as plug-in interchangeable modules in the base block. Whilst the sensor data from the module could then be processed by an Arduino microcontroller and displayed in real-time on a display screen, we wanted to develop a simpler to use PC-based interface and as such, decided to incorporate a customized MegunoLink Interface Platform dashboard.

To accomplish this, and develop additional modules, the base block was slightly modified using the free online Tinkercad software tool to firstly accommodate Arduino electronic components in the rear of the base block and secondly, to fit interchangeable sensor modules in the front (Figure 2). By plugging modules into the front cavity of the base block, it would be possible to connect to the Arduino microcontroller located at the back interior via a DB15 connector. The Arduino code to control the system functionality and the MegunoLink platform was written and uploaded to an Arduino Uno Wi-Fi Rev 2 via the Arduino integrated development environment (IDE).

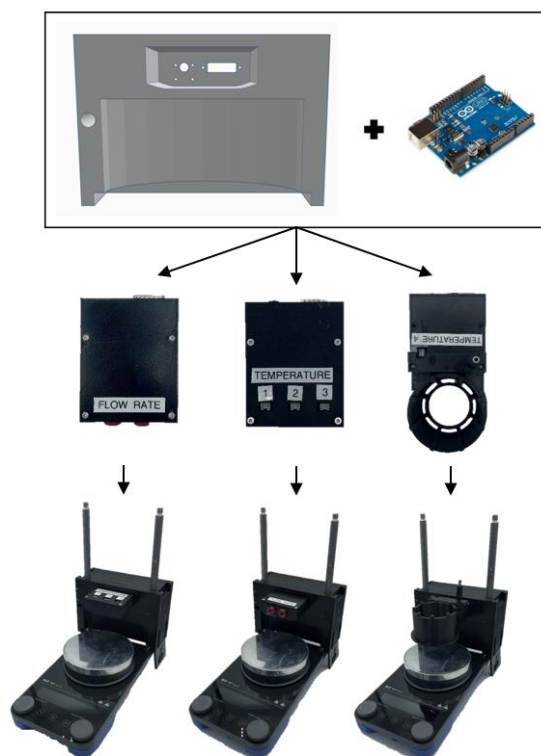


Figure 2: 3D design of continuous flow base block. Top designs correspond to the Tinkercad design of the digital system in addition to the Arduino Uno Rev 2 and bottom designs correspond to the digitized base block with the three different modules plugged in.

The sensor modules were designed to fit into the front cavity of the base but were designed to be flexible so that users could easily swap in and out different modules as desired so as to allow temperature, flow rate or other sensors to be incorporated (Figure 2). Three different modules were designed, each to perform a specific function. The first module, known as the "Temperature Module", incorporated three waterproof NTC Thermistor Temperature Adapters to simultaneously measure three different temperatures in real-time. The Phototemperature module was designed to hold a Kessil lamp to perform photochemical reactions, record temperature measurements, whilst cooling the system with compressed air and the last module was designed to measure the flow rate of the system using an SLF3C-1300F liquid flow sensor.^{23,24} Conventional liquid sensors such as these are frequently calibrated with only water and as such, the sensor was calibrated with a range of other solvents to accurately monitor their specific flow rate (Supplementary Information). The calibrated solvents were selected based on which ones were most probable to be used in reactions and were compatible with the sensor, including isopropanol (IPA), methanol, ethanol, acetone, and acetonitrile.

As well as incorporating sensors for reaction telemetry, we also wanted to be able to easily scale up the system to enable higher reactant volumes for larger-scale reactions (Figure 1C). The previous digitized system initially only allowed a maximum of 4 mL of reagent to be

manually injected into the flow path due to the use of 2 mL loops (Figure 3A), and as such, the scaled-up modular version was designed to allow for the automatic injection of up to 200 mL of reactants (Figure 3B). To achieve this, the injection block was modified to incorporate two solenoid valves at the rear that could be linked to the base block housing the Arduino microprocessor and the solvent block was modified to accommodate three Duran bottles, one 250 mL solvent reservoir bottle, and two 100 mL reactant bottles. Each bottle was pressurized with compressed gas (air/ nitrogen as desired) and connected to the two solenoid valves. Whilst the initial system for monitoring was able to incorporate a simple Arduino Uno Wifi Rev 2, the Arduino code that controls the scale-up system increased in complexity due to the addition of lines to regulate the opening and closing of the valves and as such necessitated the use of an Arduino Mega microprocessor. As the solenoid valves operate at 24 V, a solenoid shield was used to isolate the microprocessor from the current for the valves (Supplementary Information).

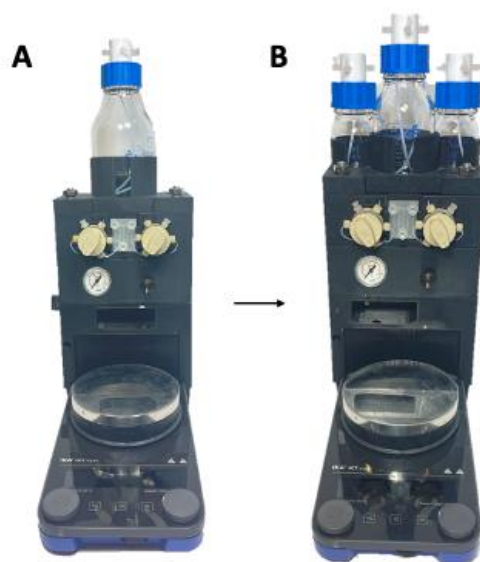


Figure 3: A) Digitised flow chemistry system on the left, B) scaled-up version of the continuous flow system on the right.

Whilst other groups digital approaches have focussed on the use of Python or Arduino screen based interfaces, we wanted to develop a simpler more familiar system for users and so elected to integrate our Arduino code and hardware with the PC interface developed by MegunoLink to allow for facile control of the system and easy visualisation of the reaction telemetry (Figure 4 and Supplementary Information).²⁵

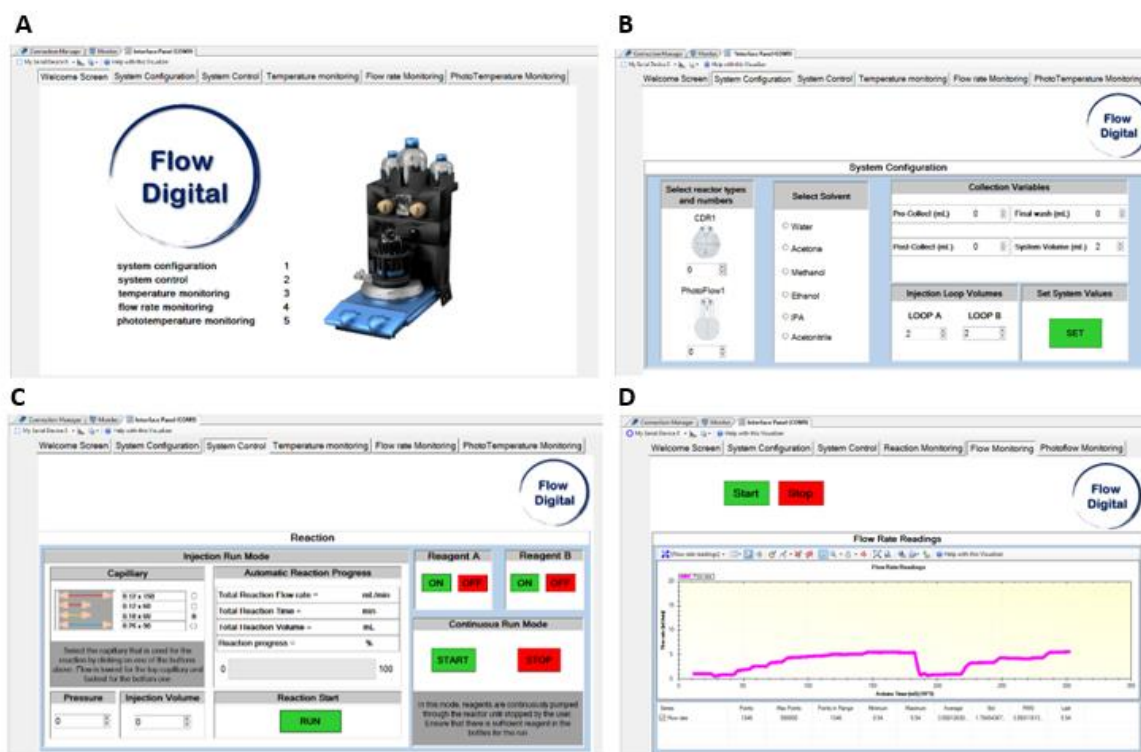


Figure 4: MegunoLink Interface of the project. A) Welcome screen tab. B) System configuration tab. C) System control tab. D) Flow rate monitoring tab.

The PC based interface was created with multiple tabs to enable the monitoring and automation of the system functionality and sensor values. The configuration tab defines how the flow system is set up (Figure 4B) allowing users to select the numbers and types of reactors, the solvent used, and the solvent collection variables. The reaction variables are defined under the control tab (Figure 4C). The factors influencing the reaction outcome are determined by the type of metal capillary used, the pressure applied to the system, and the volume of reactant that will be injected into the flow path. After these variables have been established, the Arduino code calculates how long the valves must be open for, in order for the reactants to flow using Equation 1. The flow rate and pressure correlations were measured for each solvent, resulting in different equations (Supplementary Information). In order to allow for ease of following the reaction progress for users, the Arduino code also updates the reaction output labels within the control tab by displaying a progress bar, the total volume to be collected, and the reaction's overall time and flow rate. While the equation can automate the opening and closing of the valves, the on and off buttons can also be used to manually operate them if any issues arise during a reaction run.

$$\text{Flow rate} \left(\frac{\text{volume in ml}}{\text{time in min}} \right) = a \times \text{Pressure (PSI)} + b \rightarrow \text{Time (min)} = \frac{\text{Volume (mL)}}{a \times \text{Pressure (PSI)} + b}$$

Equation 1: Flow rate and pressure linear equation where a and b are constant numbers.

The final three tabs display the sensor data for each module (Figure 4D as an example). Each tab contains a start and stop button so that the interface begins processing and displaying sensor data when the user presses the Start button. Therefore, the background noise generated by the sensor is not plotted during non-use, and only data is stored when needed.

Results and Discussion

One of the challenges in synthetic chemistry is a lack of reproducibility as a result of the plethora of reaction hardware that is available. Having noticed disparities in the literature from repeating published work in our laboratories, we wanted to design flow reactors that would provide reliable telemetry to be able to easily repeat reactions and the designed software was an essential element of that. However, it also necessitated a redesign of the Circular Disk Reactors (CDRs) (figure 5A) previously reported by the group that could easily incorporate a temperature sensor in their core to accurately monitor the temperature of the reactor and its flow path.²¹ The first digital CDR incorporated a temperature cavity within the reactor, allowing a waterproof digital temperature sensor to measure the temperature inside (Figure 5B). The second reactor was designed to monitor the solvent's actual temperature as the probe would be in direct contact with the reactor's liquid flow path (Figure 5C) enabling easy comparison of reaction telemetry. The two reactors were designed with Tinkercad and printed with polypropylene on an Ultimaker 3 3D printer using a 0.15 mm profile, 100% infill, printing temperature of 235 °C, and printing speed of 25 mm/s (Supplementary Information for further details and G-code modifications).



Figure 5: Tinkercad design illustrating reactor. A) First design of the Hilton Group. B) Modified reactor with the sensor cavity in the centre to incorporate a Digital Thermal Temperature Sensor. C) Modified reactor with the probe cavity in contact with the flow path.

Temperature analyses were carried out between a range of 30 °C to 130 °C, using different equipment covering reactor configurations, flow rates, heat blocks, and reactor designs. The digitized continuous flow system was used together with the temperature sensor module to monitor the temperature and the Flow rate module to control the flow rate of the system.

The first reactor set-up was used to evaluate the temperature variations and measurements of one CDR, whether an IKA heat block, a DrySyn heat block, with and without probe and in the absence of a heating block (Figure 6). The internal temperature of the reactor was measured with the Waterproof Digital Thermal Temperature Sensor connected to the adaptor from the Temperature module. The flow rate module was used to control the flow rate, which was set to 0.2 mL/min for all measurements.

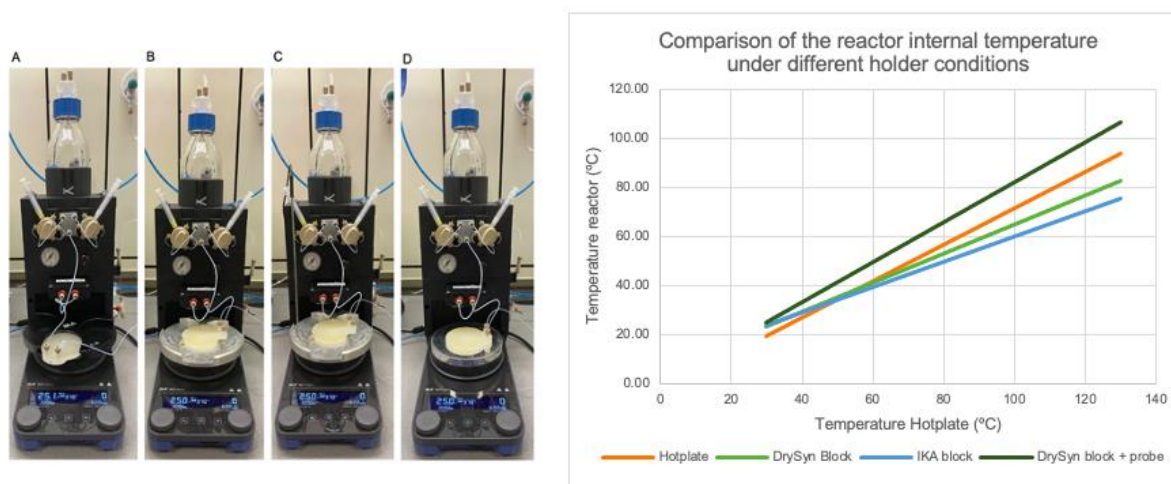



Figure 6: Temperature measurements set up. A) With the IKA Block. B) With the DrySyn Block. C) With the DrySyn Block and the temperature probe connected. D) Directly on top of the Hotplate. Graph 1: temperature variations depending on holder conditions.

The results (Figure 6), showed that the use of the DrySyn block leads to a higher internal temperature when compared to the set temperature in comparison to the IKA base. From the results it was clear that in all cases, the set temperature was lower than the internal temperature of the flow path, in some cases by as much as 60 °C, starkly illustrating the need for all chemists to record accurate temperatures of any reaction.

Further temperature analyses were carried out, using two and three CDRs connected in series at different flow rates using the IKA and DrySyn heat blocks. It was found that the heat transfer from the first reactor to the second reactor decreased as the hotplate set temperature rose. As a result, the internal temperature of the second reactor was approximately 5 °C lower than the first one. Moreover, an inverse correlation was observed between the temperature and flow rate, as the flow rate increased, the internal temperature of the reactor decreased. Surprisingly, when a third reactor was connected to the flow system, its internal temperature showed a similar behaviour that of the first reactor which we attributed to pre-heating in the second reactor. Nevertheless, according to prior data and evaluating the temperature fluctuations between the use of different heat blocks, the use of the DrySyn block allowed us

to achieve higher internal temperatures, up to 96 °C when compared to the IKA holder, which only reached 89 °C.

Up to this point, the internal temperature of the reactor had been measured but not that of the liquid within the flow channel. Using both types of reactor designs (Figure 5B, C), we were able to correlate the temperature variations between the reactor and the flow path. The measurements were performed at different flow rates using the DrySyn block.

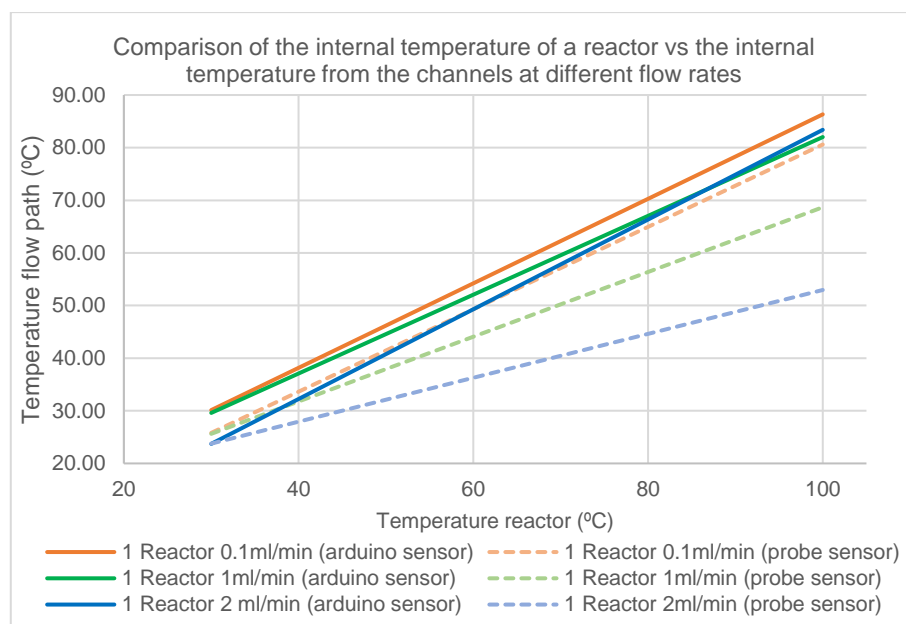


Graph 1: Correlation between the internal temperatures of a reactor and the internal temperature from the reactors channel at different flow rates.

An increase of the hotplate set temperature and flow rate led to significant temperature differences as high as 30 °C between the flow path and the reactor. However, when the temperatures of a second reactor connected in series were compared, the differences between the inner cavity and the flow path of the second reactor were not as extensive as in the first case. This result was not surprising as faster flow rates should lead to cooler reactions as the liquid takes time to heat, but this resulting graph starkly illustrates the need to accurately record the temperature of reactions for reproducibility.

Having calibrated the system and gained an understanding of the internal temperature of our CDRs, we elected to optimise a previously reported poor yielding S_NAr reaction from the group,²¹ in a reaction between 2-chloro-5-nitropyridine **1** and 4-nitrophenol **2** where we had previously used a set hotplate temperature of 65 °C, a flow rate of 0.33 mL/min with a

residence time of 26 minutes (2 CDRs). Following the temperature studies above, the reactions were carried out with the Asynt Drysyn blocks with a temperature probe attached.

Table 1, Scheme 1: Flow reaction optimisation for Scheme 1, synthesis of 5-nitro-2-(4-nitrophenoxy)pyridine (**3**).

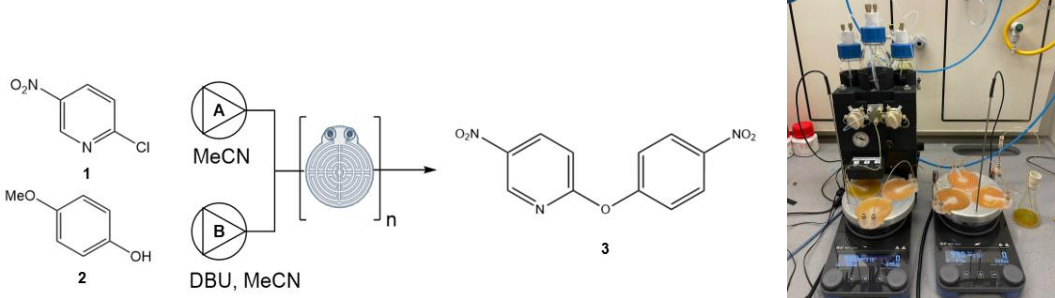


Entry	Number of CDRs	Injection Volume (mL)	Temperature Hotplate (°C)	Internal temperature CDR (°C)	Yield (%)
1	2	4	65	55	22
2	2	4	75	65	27
3	2	4	100	85	38
4	3	4	100	85	38
5	4	4	100	85	64
6	5	4	100	85	69
7	6	4	100	85	93
8	6	60	100	85	90

By monitoring the internal temperature and increasing it to 85 °C, the yield improved from 22% as previously reported to 38% as the internal temperature rose from 55 °C to 85 °C. Addition of a second hotplate, enabled the reaction path to be extended to 6 reactors (Table 1), leading to a yield of 93%. Having optimised the reaction conditions, the reaction was scaled up by loading the two 100 mL Duran bottles with the corresponding reactants. Instead of manually injecting 2 mL of the reactants into each loop, 30 mL of each solution were automatically injected into the flow path from each bottle (Table 1 Entry 8). The MegunoLink platform was used not only to monitor the reaction's flow rate and temperature but also to automate the valve opening and closing to allow reagent or solvent to flow through the system. On the configuration tab of the MegunoLink Interface, six CDRs were selected, along with acetonitrile as the solvent. The pressure applied, the capillary used, and the total injection volume were specified in the control tab. Once all the parameters were set, both valves automatically opened to allow the reactant solutions to flow through. The valves closed after 3:15 hours as determined by the equation from the Arduino code corresponding to the solvent acetonitrile, an injection volume of 60 mL using a 120 mm x 60 mm RED capillary at a pressure of 6 PSI, obtaining 2.13 g of 5-nitro-2-(4-nitrophenoxy) pyridine **3**. From the results obtained (Table 1), it was evident that this system could be used to automate scale-up reactions in an


efficient manner. Accordingly, we sought to explore two photochemical reactions in which the Phototemperature module and the scale-up system could also be used (Scheme 2 and 3).^{26,27}

Table 2, Scheme 2: Flow Photochemical synthesis of 1,2-bis(4-methoxyphenyl)-1,2-diphenylethane-1,2-diol (**5**).

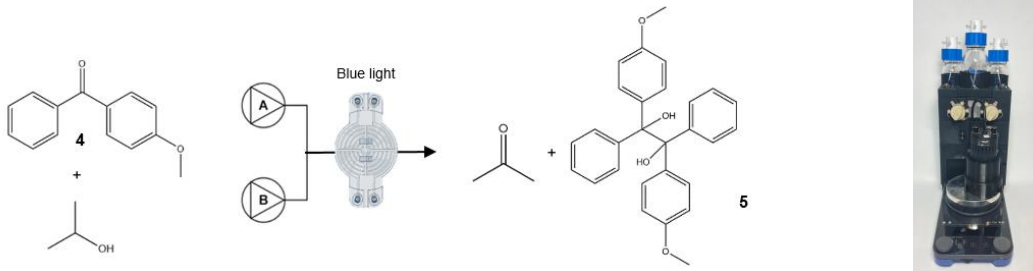

Entry	Number of CDRs	Flow rate (mL/min)	Injection Volume (mL)	Amount product obtained (g)	Yield (%)
9	1	0.1	4	0.11	60
10	1	0.06	25	0.57	81

Table 3, Scheme 3: Flow Photochemical synthesis of methyl 3-bromo-3-phenylpropanoate (**8**).

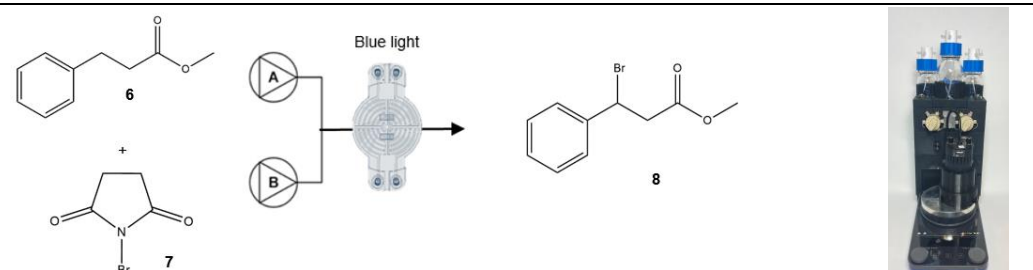

Entry	Number of CDRs	Flow rate (mL/min)	Injection Volume (mL)	Amount product obtained (g)	Yield (%)
11	1	5	4	0.43	89
12	1	5	40	2.07	85

The scale up synthesis of 1,2-bis(4-methoxyphenyl)-1,2-diphenylethane-1,2-diol (**5**) (Scheme 2) and methyl 3-bromo-3-phenylpropanoate (**8**) (Scheme 3) were successfully obtained using the Phototemperature module. Both reactions were performed with one CDR placed 30 mm below a blue light lamp while being air cooled. Further details of these reactions can be found in the supplementary information as well as the 3D printed parts of the system, the Arduino code and MegunoLink interface platform calibrations. In each case, the reaction was also scaled up using the MegunoLink software enabling injection volumes of 25 mL and 40 mL respectively, with comparable yields in each case. For the diol (**5**) we reduced the flow rate to 0.06 mL/min from 0.1 mL/min which led to an increased yield of the scaled up reaction.

Conclusions

In summary, three innovative technologies have been combined: continuous flow chemistry, 3D printing, and open-source software to design a low-cost 3D-printed continuous flow chemistry system digitized with Arduino open-source electronics. The MegunoLink PC interface simplified the monitoring and reporting of the sensor data and the control of the system functionality. The extensive tools and services available in the software platform enabled the design of a customized dashboard according to the project's requirements.

The development of this system provides a clear understanding of how to accurately monitor system parameters in order to effectively report flow chemical reactions. Furthermore, the affordability of 3D printing technologies and Arduino electronics allows for the standardization of flow chemical synthesis and the expansion of its applications in a low-cost digital platform and additional low-cost approaches to flow chemistry will be reported in due course.

Additional Resources

Full Arduino code and installation files are available from Github: [GitHub - sthilton/Proteus-Flow-Digital](https://github.com/sthilton/Proteus-Flow-Digital). Supporting Information includes detailed CAD designs for all parts of the system.

References

- 1) a) Plutschack M.B., Pieber B., Gilmore K., Seeberger P.H., The Hitchhiker's Guide to Flow Chemistry *Chemical Reviews*. **2017**, *117*, 11796–893; b) König B., Kreitmeier P., Hilgers P., Wirth T., Flow Chemistry in Undergraduate Organic Chemistry Education. *J. Chem. Educ.* **2013**, *90*, 934–936; c) Andrea Laybourn A., Robertson K., Slater A.G., Quid Pro Flow. *Journal of the American Chemical Society* **2023**, *145*, 4355-4365; d) Seifrid M., Pollice R., Aguilar-Granda A., Chan Z. M., Hotta K., Ser C. T., Vestfrid J., Wu T. C., Aspuru-Guzik A., Autonomous Chemical Experiments: Challenges and Perspectives on Establishing a Self-Driving Lab. *Accounts of Chemical Research* **2022**, *55*, 2454-2466; e) May, S. A. Flow Chemistry, Continuous Processing, and Continuous Manufacturing: A Pharmaceutical Perspective. *J.*

- Flow Chem.* **2017**, *7*, 137–145; f) Movsisyan, M., Delbeke, E. I. P., Berton, J. K. E.T., Battilocchio, C., Ley, S. V., Stevens, C. V. Taming hazardous chemistry by continuous flow technology. *Chem. Soc. Rev.* **2016**, *45*, 4892–4928; g) Gutmann, B., Cantillo, D., Kappe, C. O. Continuous-Flow Technology – A Tool for the Safe Manufacturing of Active Pharmaceutical Ingredients. *Angew. Chem., Int. Ed.* **2015**, *54*, 6688–6728; h) Hartman, R. L., McMullen, J. P., Jensen, K. F. Deciding Whether To Go with the Flow: Evaluating the Merits of Flow Reactors for Synthesis. *Angew. Chem., Int. Ed.* **2011**, *50*, 7502–7519.
- 2) a) Alvarez E, Romero-Fernandez M, Iglesias D, Martinez-Cuenca R, Okafor O, Delorme A, *et al.* Electrochemical Oscillatory Baffled Reactors Fabricated with Additive Manufacturing for Efficient Continuous-Flow Oxidations. *ACS Sustain Chem Eng.* **2022**, *10*, 2388–2396; b) Renner M., Griesbeck A., Think and Print: 3D Printing of Chemical Experiments. *J Chem Educ.* **2020**, *97*, 3683–3689; c) Harding M. J., Brady S., O’Connor H., Lopez-Rodriguez R., Edwards M.D., Tracy S., *et al.* 3D printing of PEEK reactors for flow chemistry and continuous chemical processing. *React Chem Eng.* **2020** *5*, 728–735; d) Sans V. Emerging trends in flow chemistry enabled by 3D printing: Robust reactors, biocatalysis and electrochemistry. Vol. 25, *Current Opinion in Green and Sustainable Chemistry*. Elsevier B.V.; **2020**; e) Xu X., Zhang M., Jiang P., Liu D., Wang Y., Xu X., *et al.* Direct ink writing of Pd-Decorated Al₂O₃ ceramic based catalytic reduction continuous flow reactor. *Ceram Int.* **2022**, *48*, 10843–10851; f) Capel A. J., Rimington R. P., Lewis M. P. *et al.* 3D printing for chemical, pharmaceutical and biological applications. *Nat Rev Chem* **2018**, *2*, 422–436.
- 3) a) Gong H., Woolley A. T., Nordin G. P. High density 3D printed microfluidic valves, pumps, and multiplexers HHS Public Access. *Lab Chip.* **2016**, *16*, 2450–2458; b) Gordeev E. G., Erokhin K. S., Kobelev A.D., Burykina J., Novikov P., Ananikov V. P. Exploring metallic and plastic 3D printed photochemical reactors for customizing chemical synthesis. *Sci Rep.* **2022**, *12*, 3780; c) Lee H. J., Roberts R. C., Im D. J., Yim S. J., Kim H., Kim J. T., *et al.* Enhanced Controllability of Fries Rearrangements Using High-Resolution 3D-Printed Metal Microreactor with Circular Channel. *Small.* **2019** *15*, 1905005; d) Rastelli E. J., Yue D., Millard C., Wipf P. 3D-printed cartridge system for in-flow photo-oxygenation of 7-aminothienopyridinones. *Tetrahedron.* **2021**, *79*, 131875; e) Capel A. J., Edmondson S., Christie S. D. R., Goodridge R. D., Bibb

- R. J., Thurstans M. Design and additive manufacture for flow chemistry. *Lab Chip*. **2013**, *13*, 4583–4590; f) Gutmann B., Köckinger M., Glotz G., Ciaglia T., Slama E., Zadavec M., *et al.* Design and 3D printing of a stainless steel reactor for continuous difluoromethylations using fluoroform. *React Chem Eng*. **2017**, *2*, 919–927; g) Neumaier J. M., Madani A., Klein T., Ziegler T. Low-budget 3D-printed equipment for continuous flow reactions. *Beilstein Journal of Organic Chemistry*. **2019**, *15*, 558–566; h) Maier M. C., Valotta A., Hiebler K., Soritz S., Gavric K., Grabner B., *et al.* 3D Printed Reactors for Synthesis of Active Pharmaceutical Ingredients in Continuous Flow. *Org Process Res Dev*. **2020**, *24*, 2197–2207.
- 4) Rao Z. X., Patel B., Monaco A., Cao Z., Barniol-Xicota M., Pichon E., *et al.* 3D-Printed Polypropylene Continuous-Flow Column Reactors: Exploration of Reactor Utility in SNAr Reactions and the Synthesis of Bicyclic and Tetracyclic Heterocycles. *European J. Org. Chem*. **2017**, **2017**, *44*, 499–504.
- 5) Maier M. C., Lebl R., Sulzer P., Lechner J., Mayr T., Zadavec M., *et al.* Development of customized 3D printed stainless steel reactors with inline oxygen sensors for aerobic oxidation of Grignard reagents in continuous flow. *React Chem Eng*. **2019**, *4*, 393–401.
- 6) a) Lake J. R., Heyde K.C., Ruder W.C. Low-cost feedback-controlled syringe pressure pumps for microfluidics applications. *PLoS One*. **2017**, *12*, 0175089; b) Menzel F., Klein T., Ziegler T., Neumaier J.M. 3D-printed PEEK reactors and development of a complete continuous flow system for chemical synthesis. *React Chem Eng*. **2020**, *5*, 1300–1310; c) Baas S., Saggiomo, V., Ender3 3D printer kit transformed into open, programmable syringe pump set, *Hardware X*, **2021**, *10*, e00219; d) Iannone M., Caccavo D., Barba A. A., Lamberti G., A low-cost push–pull syringe pump for continuous flow applications, *Hardware X*, **2022**, *11*, e00295; e) Rogosic R., Poloni M., Marroquin-Garcia R., Dimech D., Passariello Jansen J., Cleij T.J., Eersels K., van Grinsven B., Diliën H. Cost-effective, scalable and smartphone-controlled 3D-Printed syringe pump - From lab bench to point of care biosensing applications, *Physics in Medicine*, **2022**, *14*, 100051; f) Tsuda S., Jaffery H.; ,Doran D., Hezwani M., Robbins P. J., Yoshida M., Cronin L. Customizable 3D Printed ‘Plug and Play’ Millifluidic Devices for Programmable Fluidics *PLOS One* **2015**, *10*, e0141640; g) Dragone V., Sans V., Rosnes M.H., Kitson P.J., Cronin L. 3D-printed devices

- for continuous-flow organic chemistry. *Beilstein Journal of Organic Chemistry*. **2013** 9, 951–859; h) Menzel, F., Cotton, J., Klein, T., Maurer, A., Ziegler, T., & Neumaier, J. M. FOMSy: 3D-printed flexible open-source microfluidic system and flow synthesis of PET-tracer. *Journal of Flow Chemistry*. **2023**, <https://doi.org/10.1007/s41981-023-00267-z>.
- 7) Prabhu G. R. D, Urban P. L., Elevating Chemistry Research with a Modern Electronics Toolkit. *Chem Rev.* **2020**, 120, 9482–553.
 - 8) Magaraci M. S., Bermudez J. G., Yogish D., Pak D. H., Mollov V., Tycko J., *et al.* Toolbox for Exploring Modular Gene Regulation in Synthetic Biology Training. *ACS Synth Biol.* **2016**, 5, 50.
 - 9) Ghosh S., Aggarwal K., U V. T., Nguyen T., Han J., Ahn C.H. A new microchannel capillary flow assay (MCFA) platform with lyophilized chemiluminescence reagents for a smartphone-based POCT detecting malaria. *Microsystems & Nanoengineering*, **2020**, 6, 5.
 - 10) di Caprio G., Stokes C., Higgins J. M., Schonbrun E., Weitz D. A. Single-cell measurement of red blood cell oxygen affinity. *Proc Natl Acad Sci.* **2015**, 112, 9984–9989.
 - 11) Le C. C., Wismer M. K., Shi Z. C., Zhang R., Conway D., Li G., *et al.* A General Small-Scale Reactor to Enable Standardization and Acceleration of Photocatalytic Reactions. *ACS Cent Sci.* **2017**, 3, 647–653.
 - 12) Fitzpatrick D. E., O'Brien M., Ley S. V. A tutored discourse on microcontrollers, single board computers and their applications to monitor and control chemical reactions. *React Chem Eng.* **2020**, 5, 201–220.
 - 13) White J. A., Streets A.M. Controller for microfluidic large-scale integration. *HardwareX.* **2018**, 3, 135–145.
 - 14) Longwell S.A., Fordyce P.M. MicrIO: An open-source autosampler and fraction collector for automated microfluidic input-output. *Lab Chip.* **2020**, 20, 93–106.
 - 15) Fitzpatrick D.E., Maujean T., Evans A. C., Ley S. V. Across-the-World Automated Optimization and Continuous-Flow Synthesis of Pharmaceutical Agents Operating Through a Cloud-Based Server. *Angewandte Chemie.* **2018**, 130, 15348–15352.

- 16) Fitzpatrick D.E., Battilocchio C., Ley S. V. A Novel Internet-Based Reaction Monitoring, Control and Autonomous Self-Optimization Platform for Chemical Synthesis. *Org Process Res Dev.* **2016**, *20*, 386–94.
- 17) Cardoso R. M., dos Santos R. O., Munoz R. A. A., Garcia C. D., Blanes L. A multi-pump magnetohydrodynamics lab-on-a-chip device for automated flow control and analyte delivery. *Sensors* **2020**, *20*, 1–9.
- 18) Mijalis A. J., Thomas D. A., Simon M. D., Adamo A., Beaumont R., Jensen K. F., *et al.* A fully automated flow-based approach for accelerated peptide synthesis. *Nat Chem Biol.* **2017**, *13*, 464–466.
- 19) Kim T. H., Hahn Y.K., Lee J., van Noort D., Kim M. S. Solenoid Driven Pressure Valve System: Toward Versatile Fluidic Control in Paper Microfluidics. *Anal Chem.* **2018**, *90*, 2534–2541.
- 20) Ingham R.J., Battilocchio C., Hawkins J.M., Ley S. V. Integration of enabling methods for the automated flow preparation of piperazine-2-carboxamide. *Beilstein Journal of Organic Chemistry.* **2014**, *12*; 641–652.
- 21) Penny M. R, Rao Z. X, Peniche B. F, Hilton S. T. Modular 3D Printed Compressed Air Driven Continuous-Flow Systems for Chemical Synthesis. *European J Org Chem.* **2019**, *23*, 3783–3787.
- 22) a) Penny M. R, Hilton S.T. Design and Development of 3D Printed Catalytically Active Stirrers for Chemical Synthesis. *React. Chem. Eng.* **2020**, *5*, 853–858; b) Penny M. R., Tsui N., Hilton, S.T. Extending practical flow chemistry into the undergraduate curriculum via the use of a portable low-cost 3D printed continuous flow system. **2021**, *J Flow Chem* *11*, 19–29; c) Penny M. R, Rao Z. X, Thavarajah R., Ishaq A., Bowles B. J., Hilton S. T. 3D printed tetrakis(triphenylphosphine)palladium (0) impregnated stirrer devices for Suzuki–Miyaura cross-coupling reactions *React. Chem. Eng.*, **2023**, *8*, 752–757.
- 23) SLF3C-1300F - Next generation in liquid flow sensing up to 40 ml/min and TC feature, Available from: <https://sensirion.com/products/catalog/SLF3C-1300F/>, accessed 10th April 2023.
- 24) a) Walmsley L, Hilton S.T., Sellier E, Penny M, Maddox D. Control and Monitoring of Temperature in 3D-Printed Circular Disk Reactors for Continuous Flow Photochemistry using Raspberry Pi Based Software. *ChemRxiv* **2021**, 10.26434/chemrxiv-2021-cxs25; b) Penny M, Hilton S. 3D Printed Reactors and

Kessil Lamp Holders for Flow Photochemistry: Design and System Standardization . ChemRxiv. **2021**, 10.26434/chemrxiv-2021-kmxgd.

25) <https://www.megunolink.com/> Accessed 8th April 2023.

26) Kate Volpe, K. and Podlesny E. E. *J. Chem. Educ.* **2020**, 97, 586–591.

27) Cantillo D., de Frutos O., Rincon J. A., Mateos C., Kappe C.O. A Scalable Procedure for Light-Induced Benzylic Brominations in Continuous Flow. *J Org Chem.* **2014**, 79, 223–229.